



PHIL

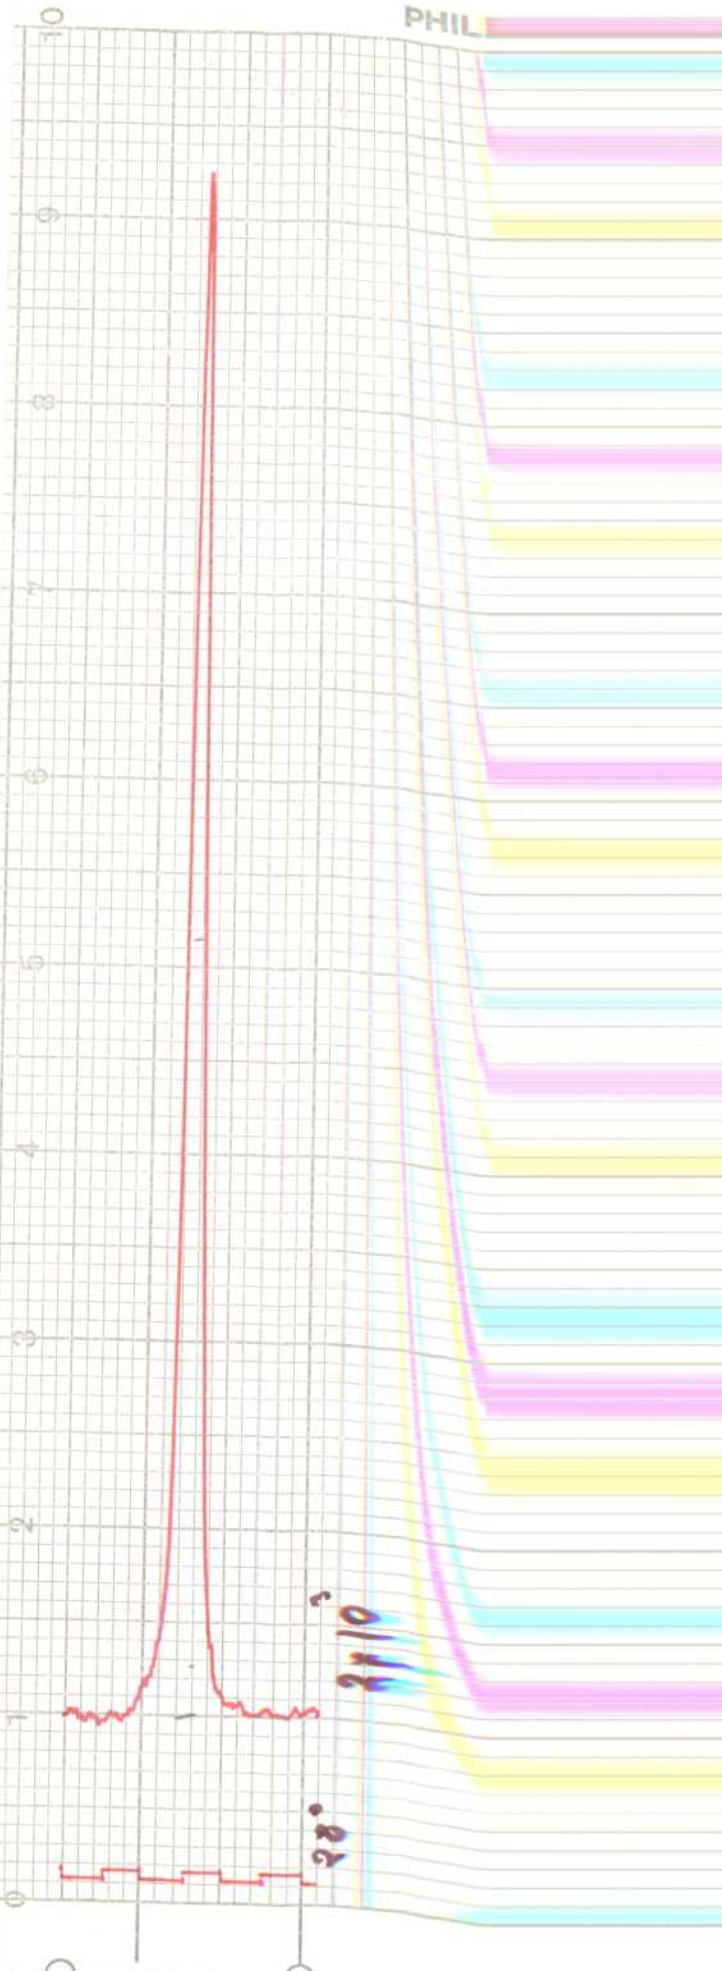

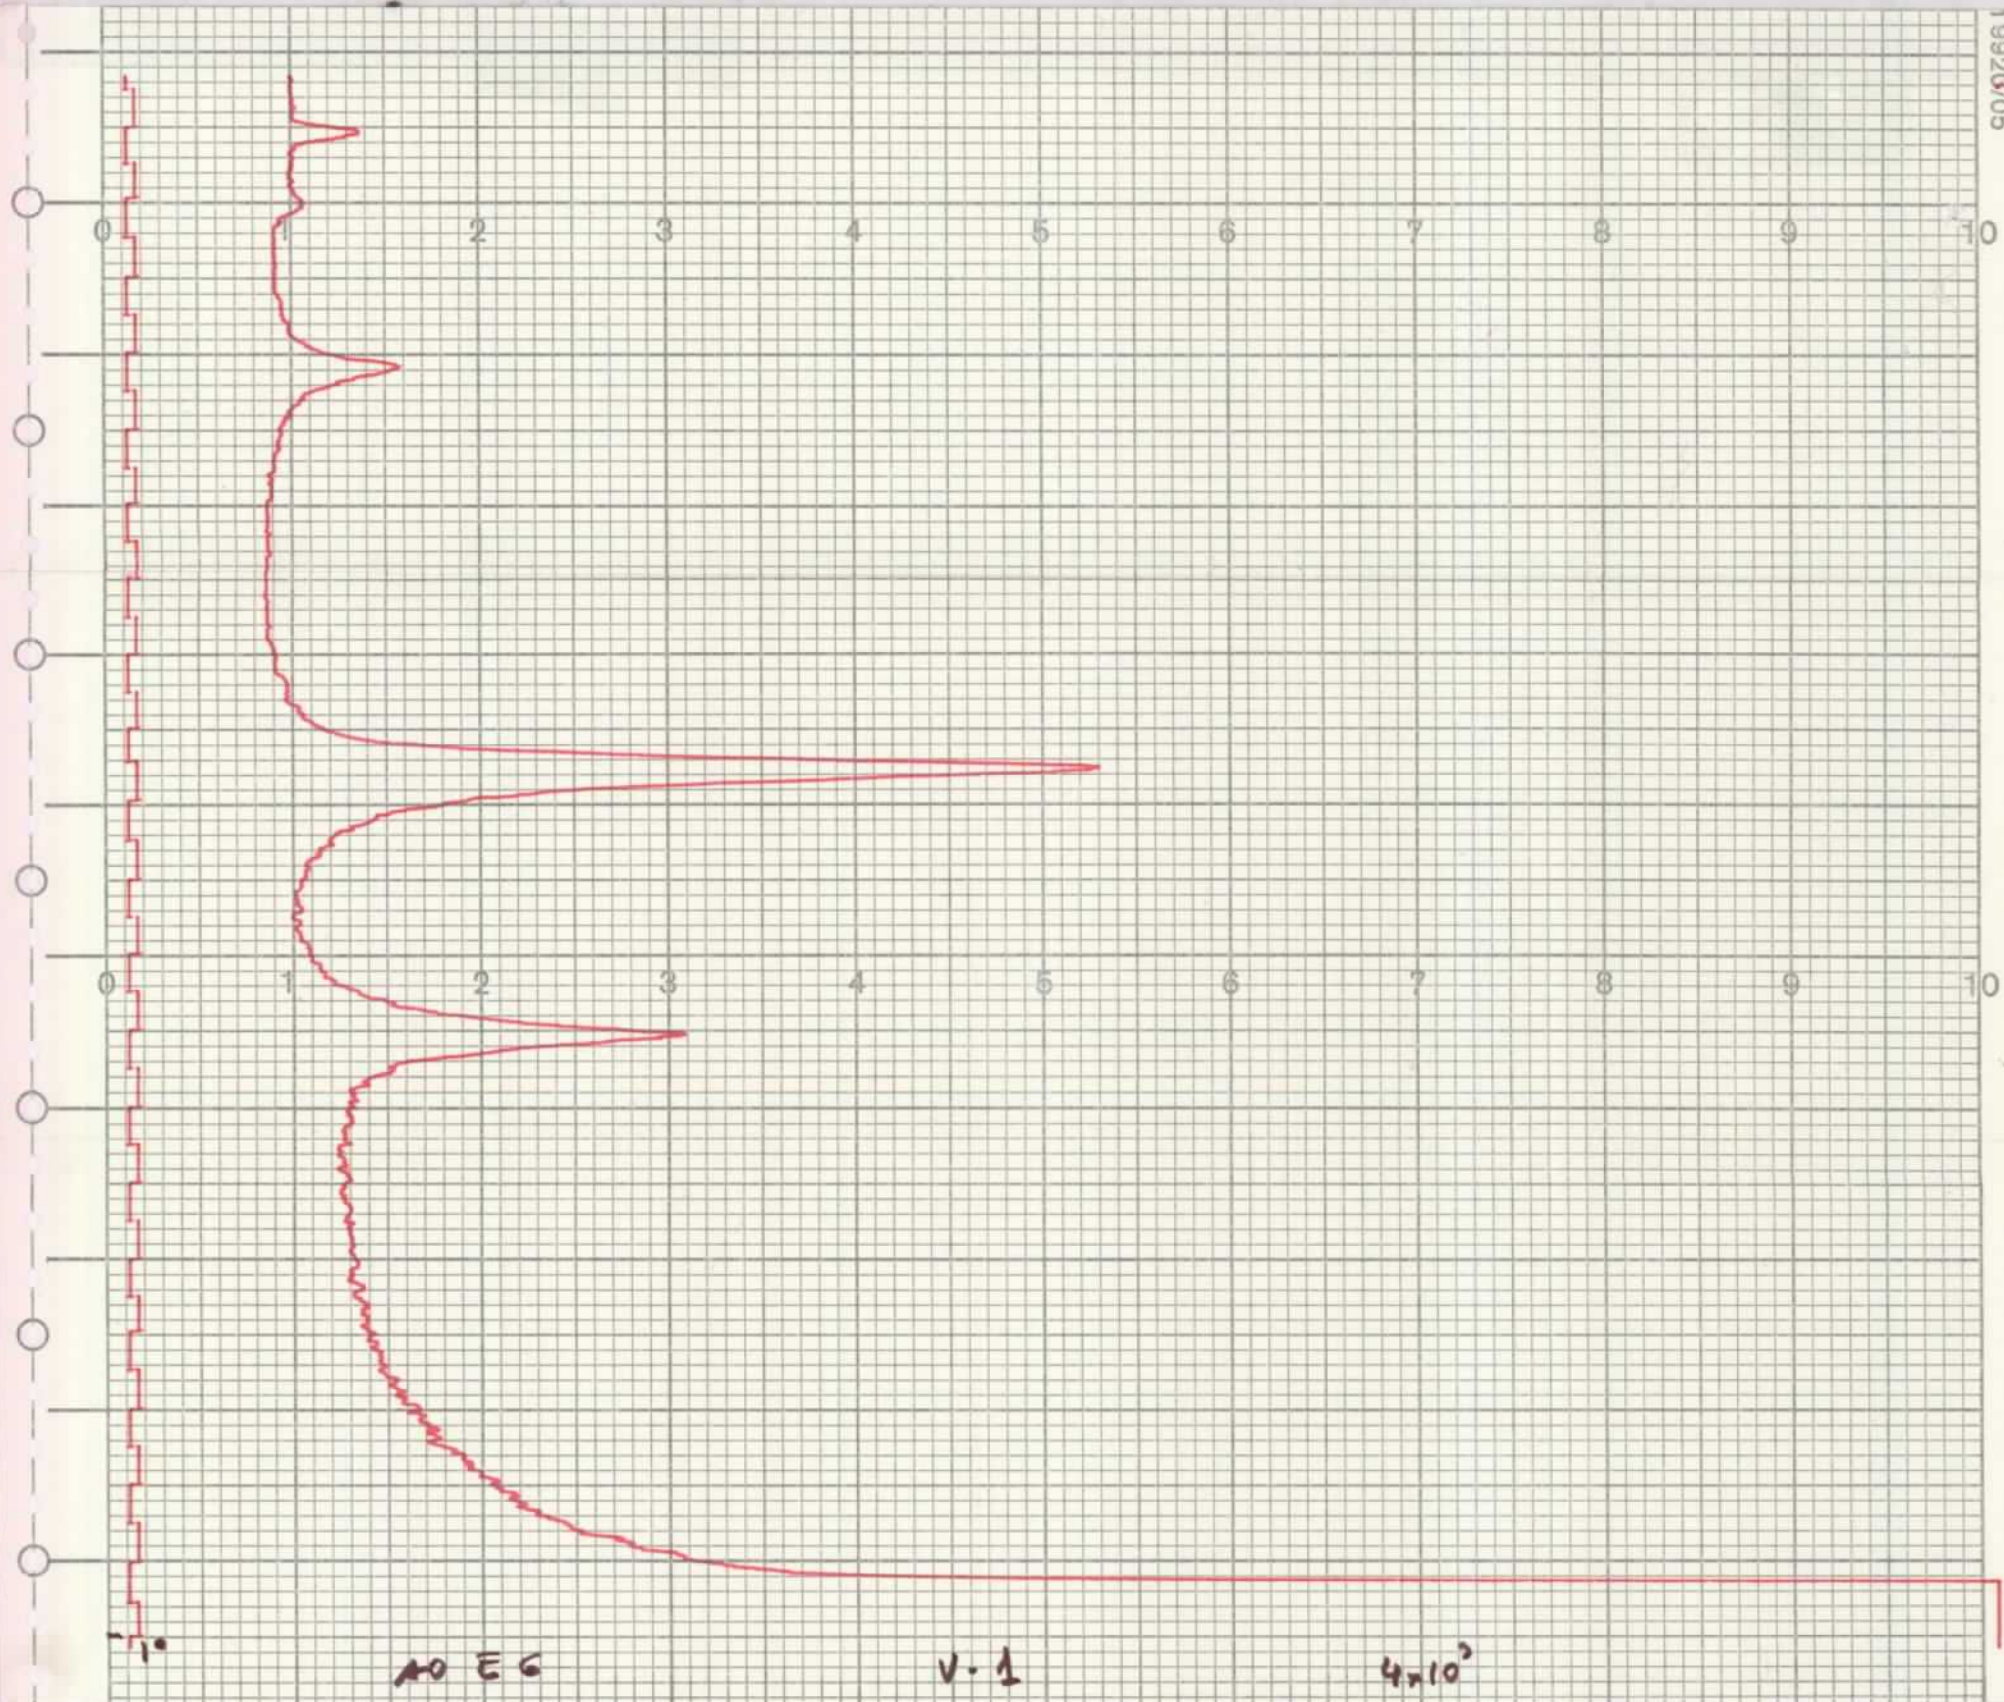


10

AD ECG

V-1


4×10^2

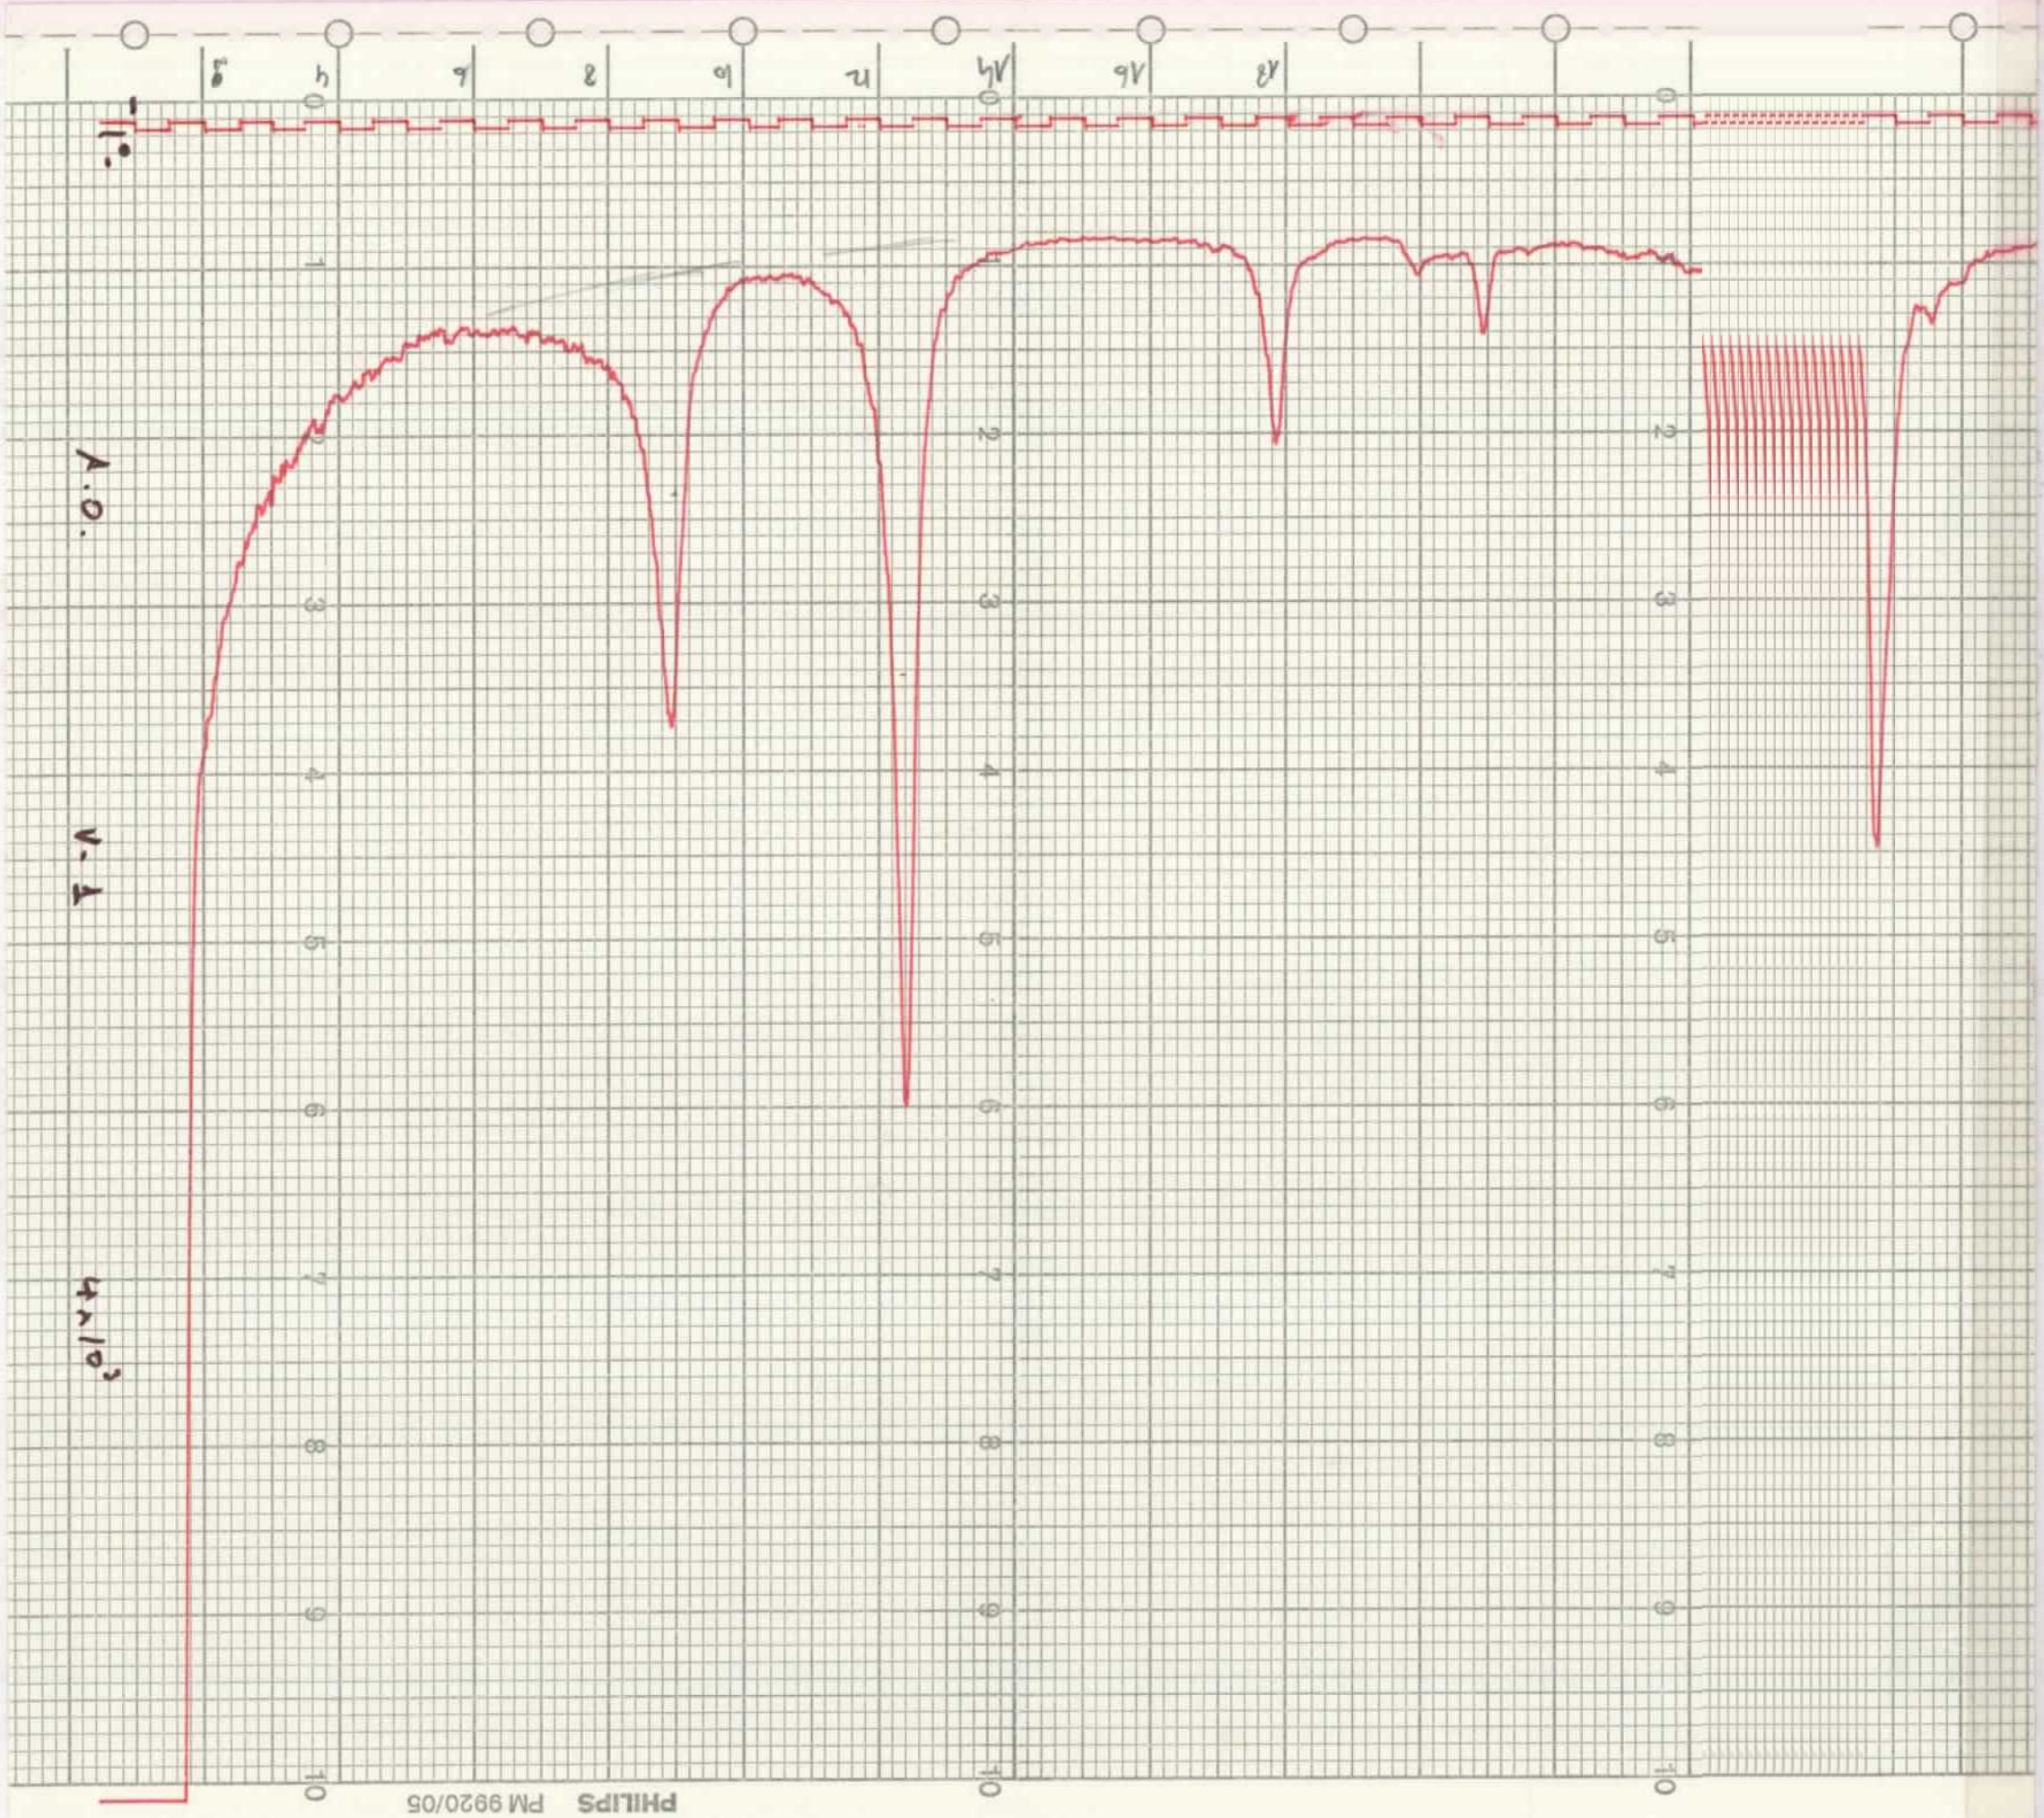



A.O.


V.A

4×10^3

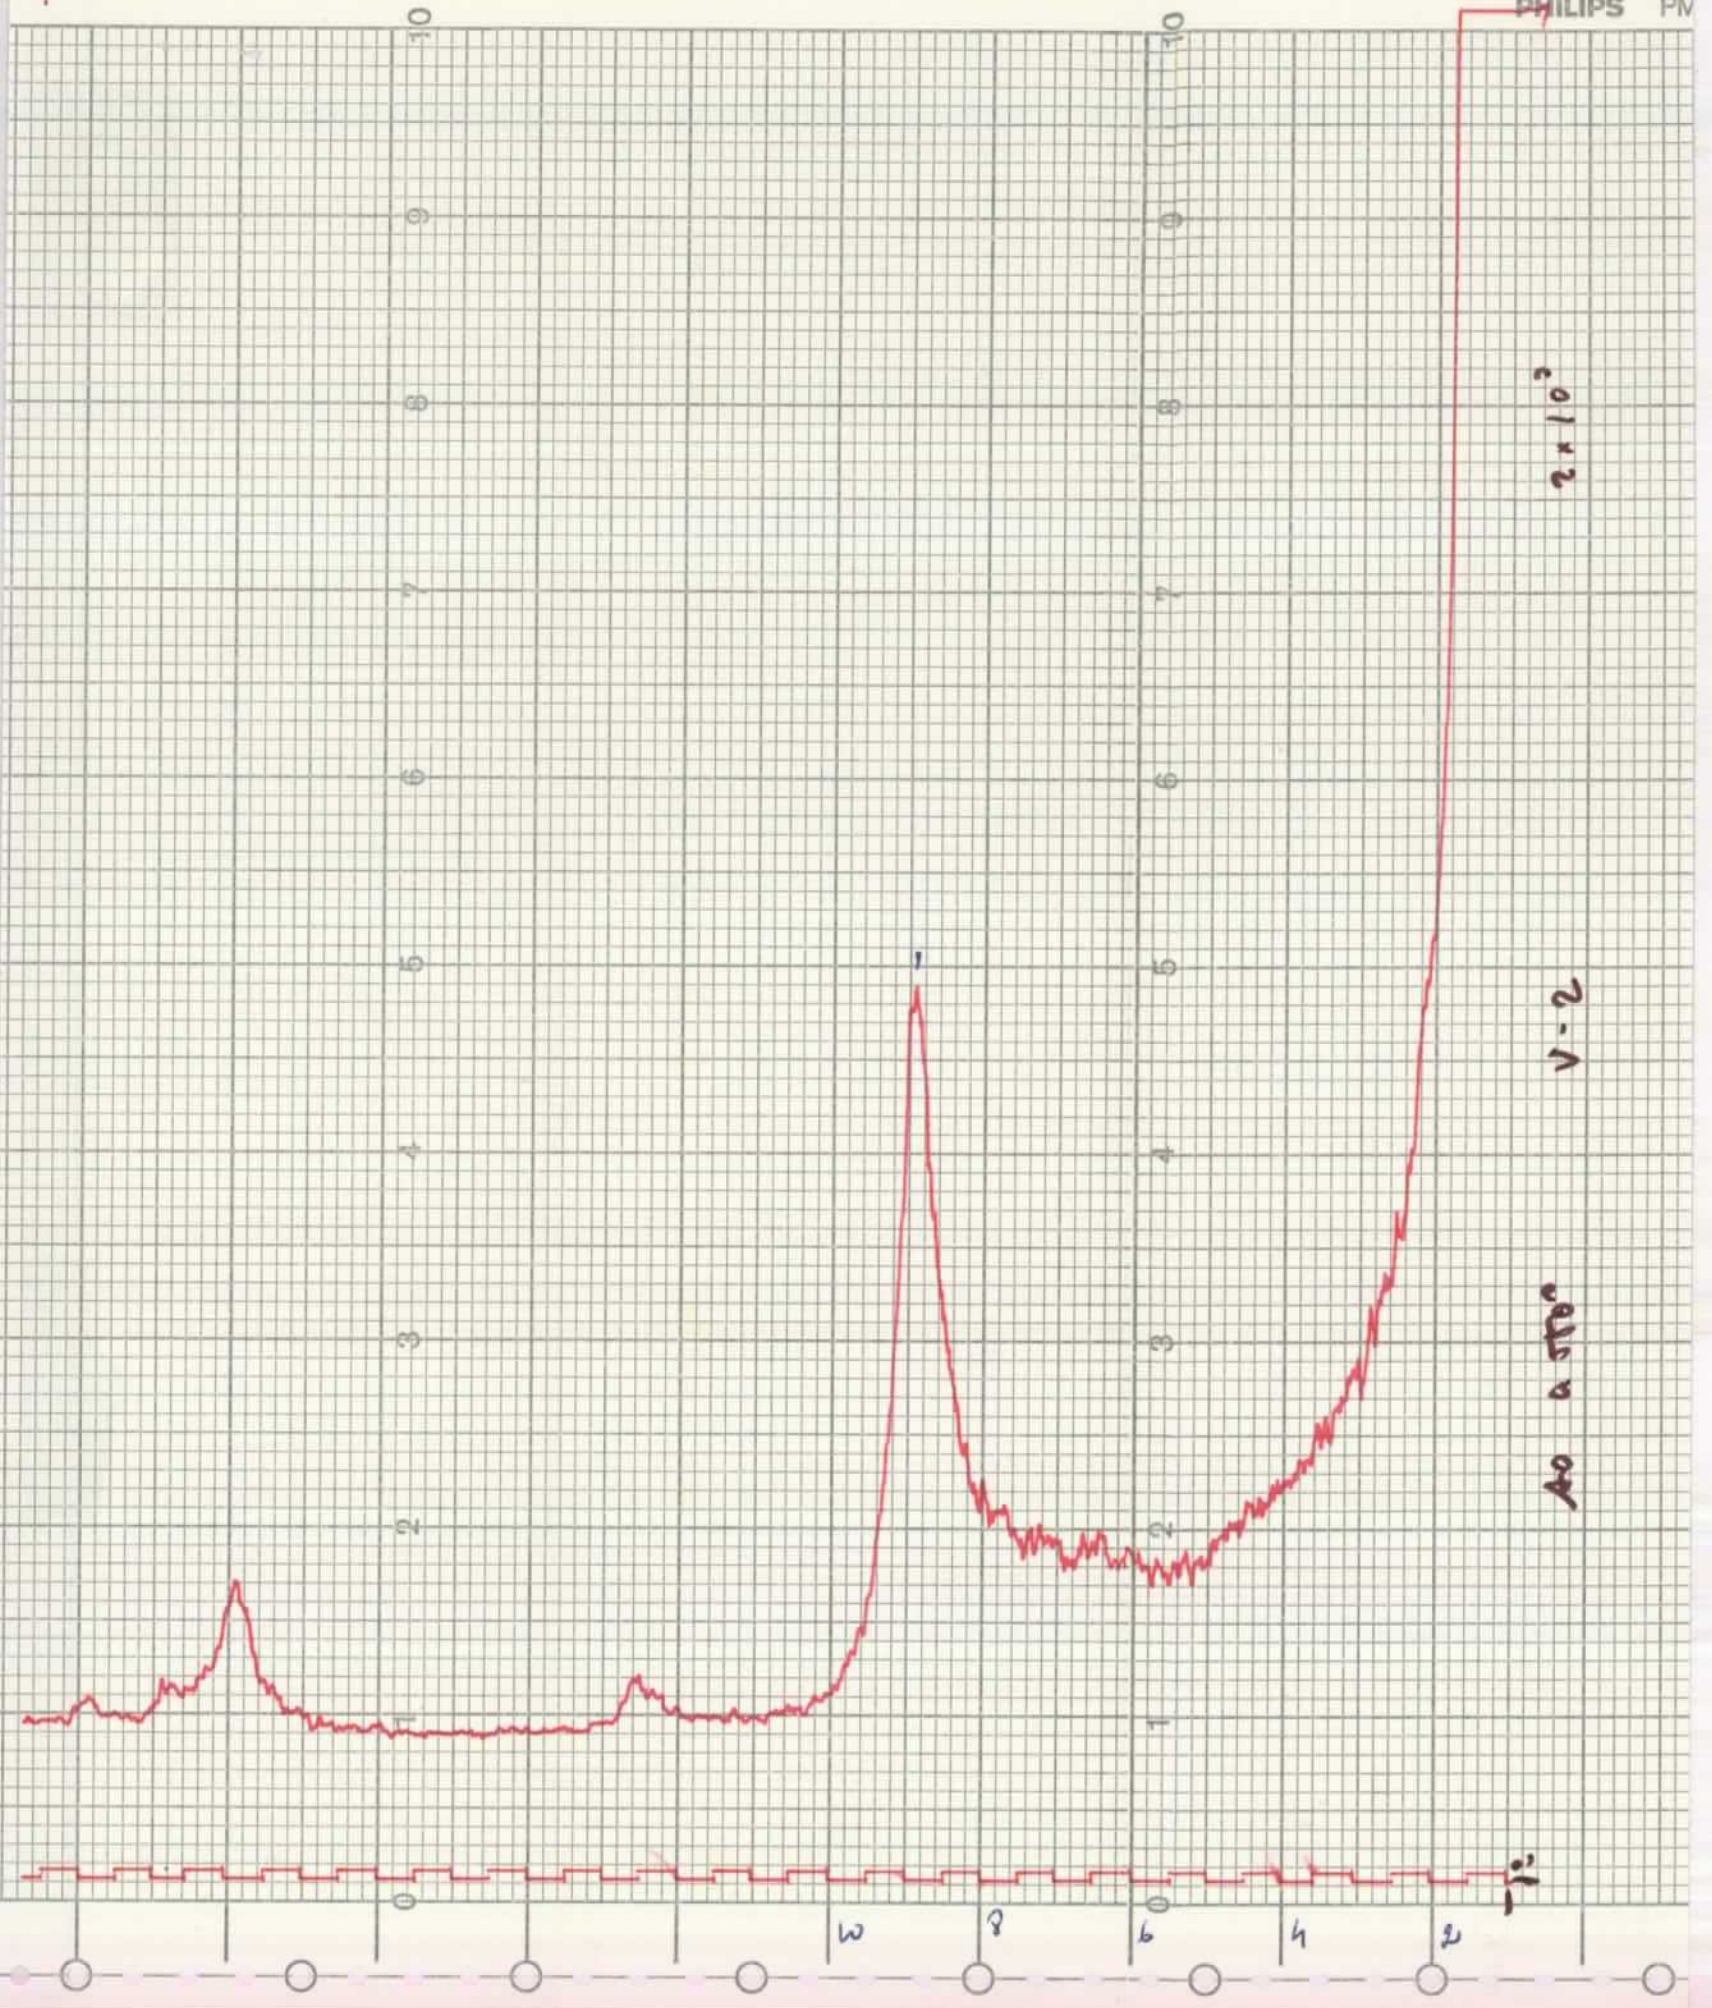

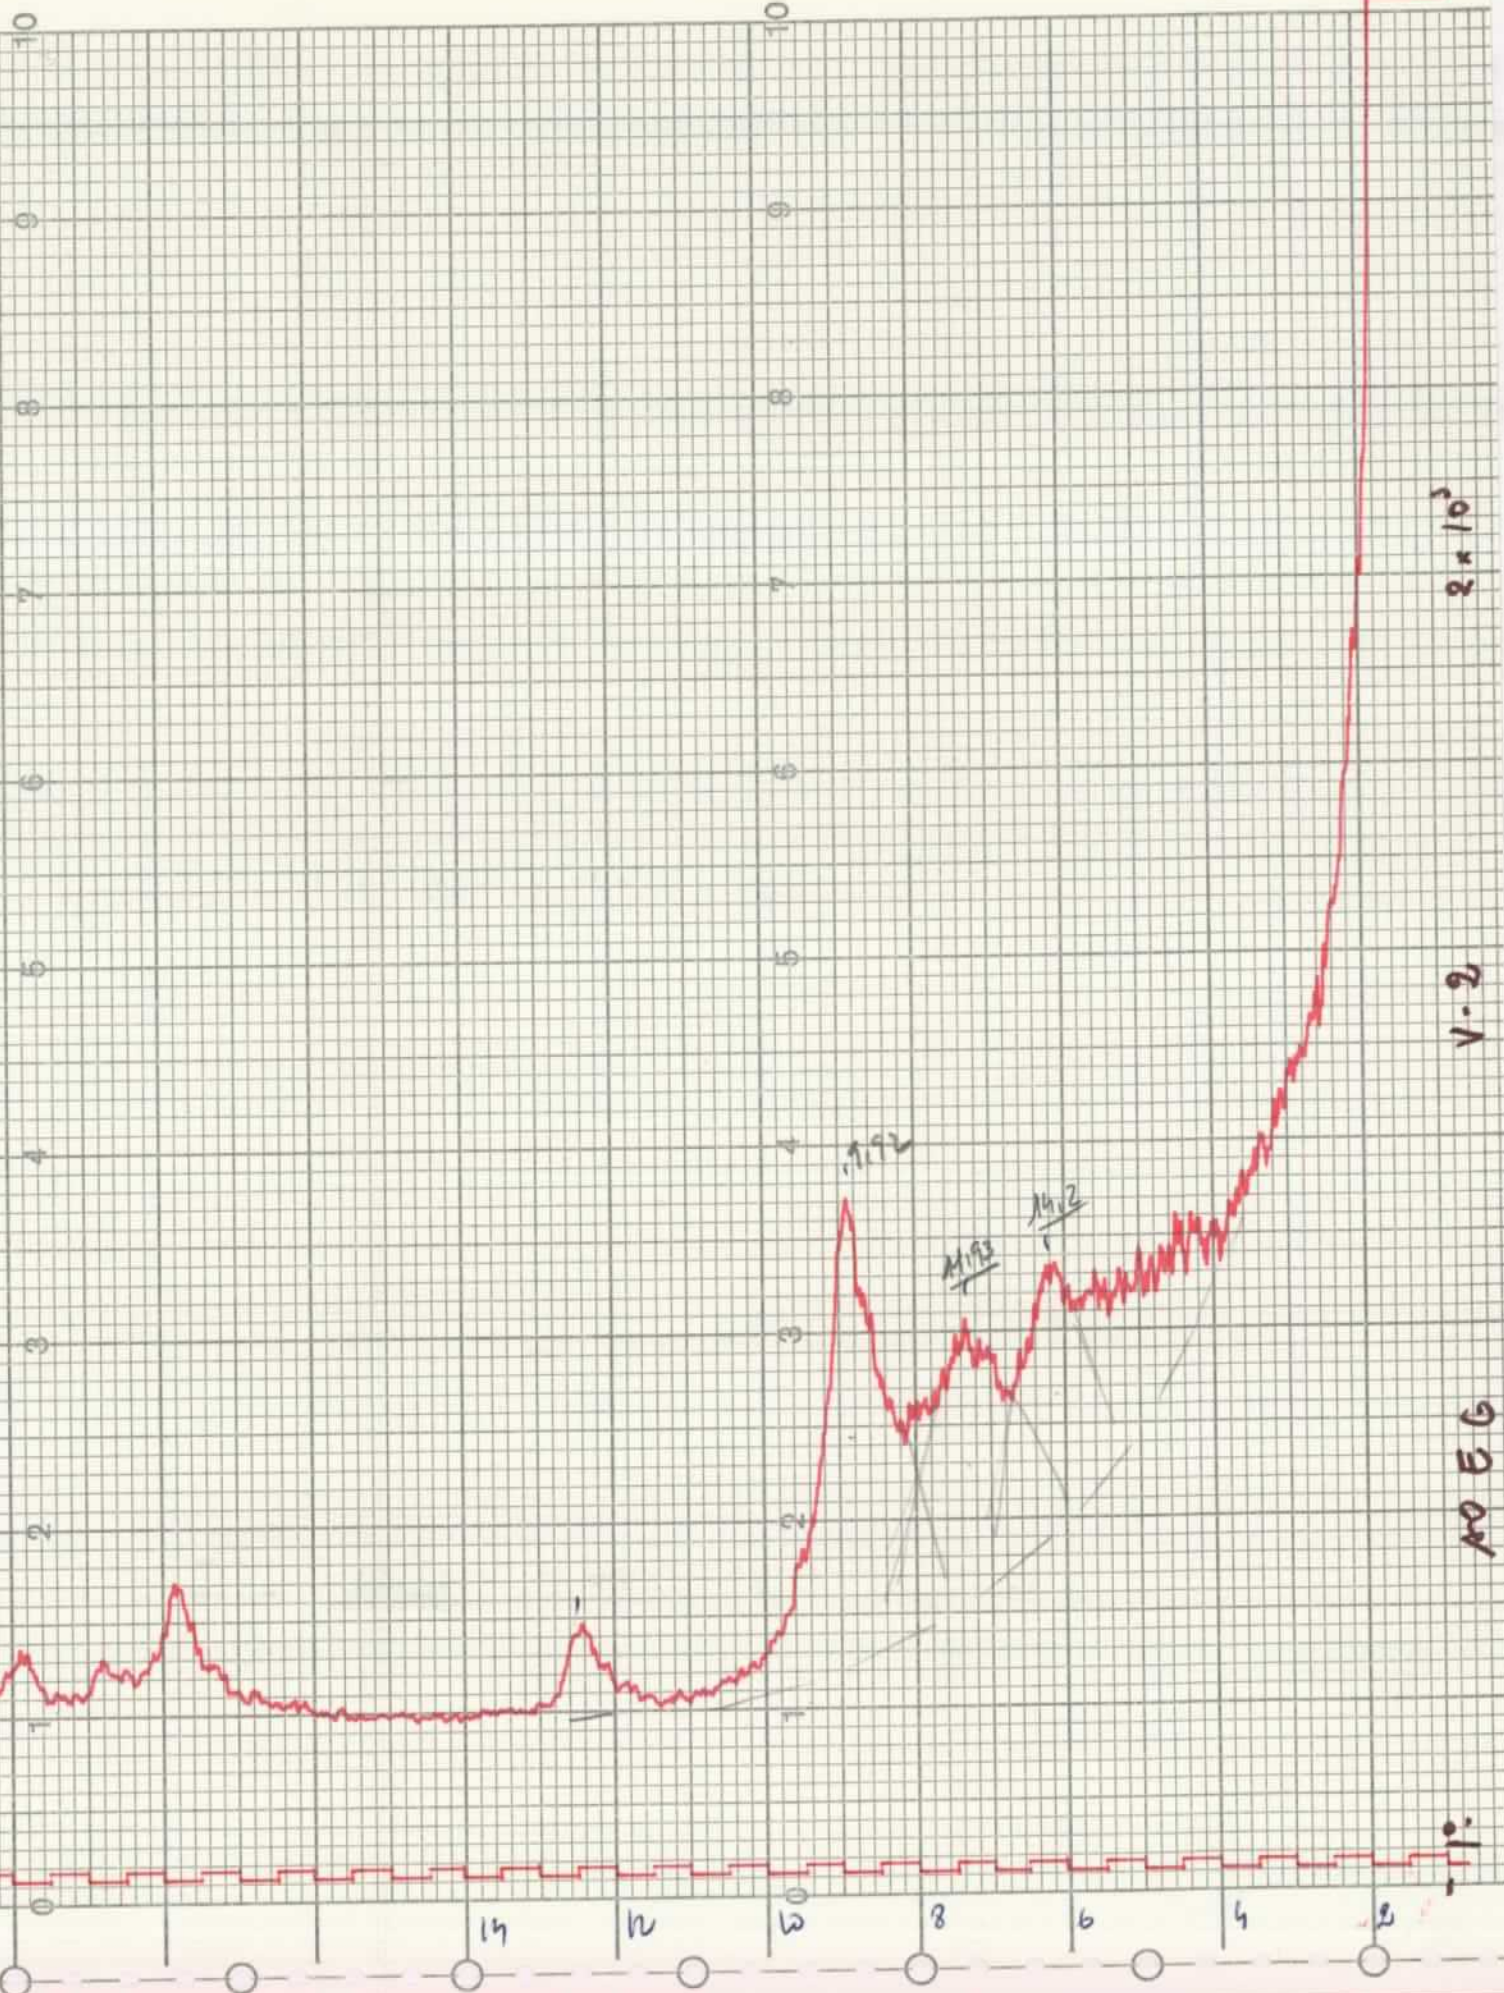

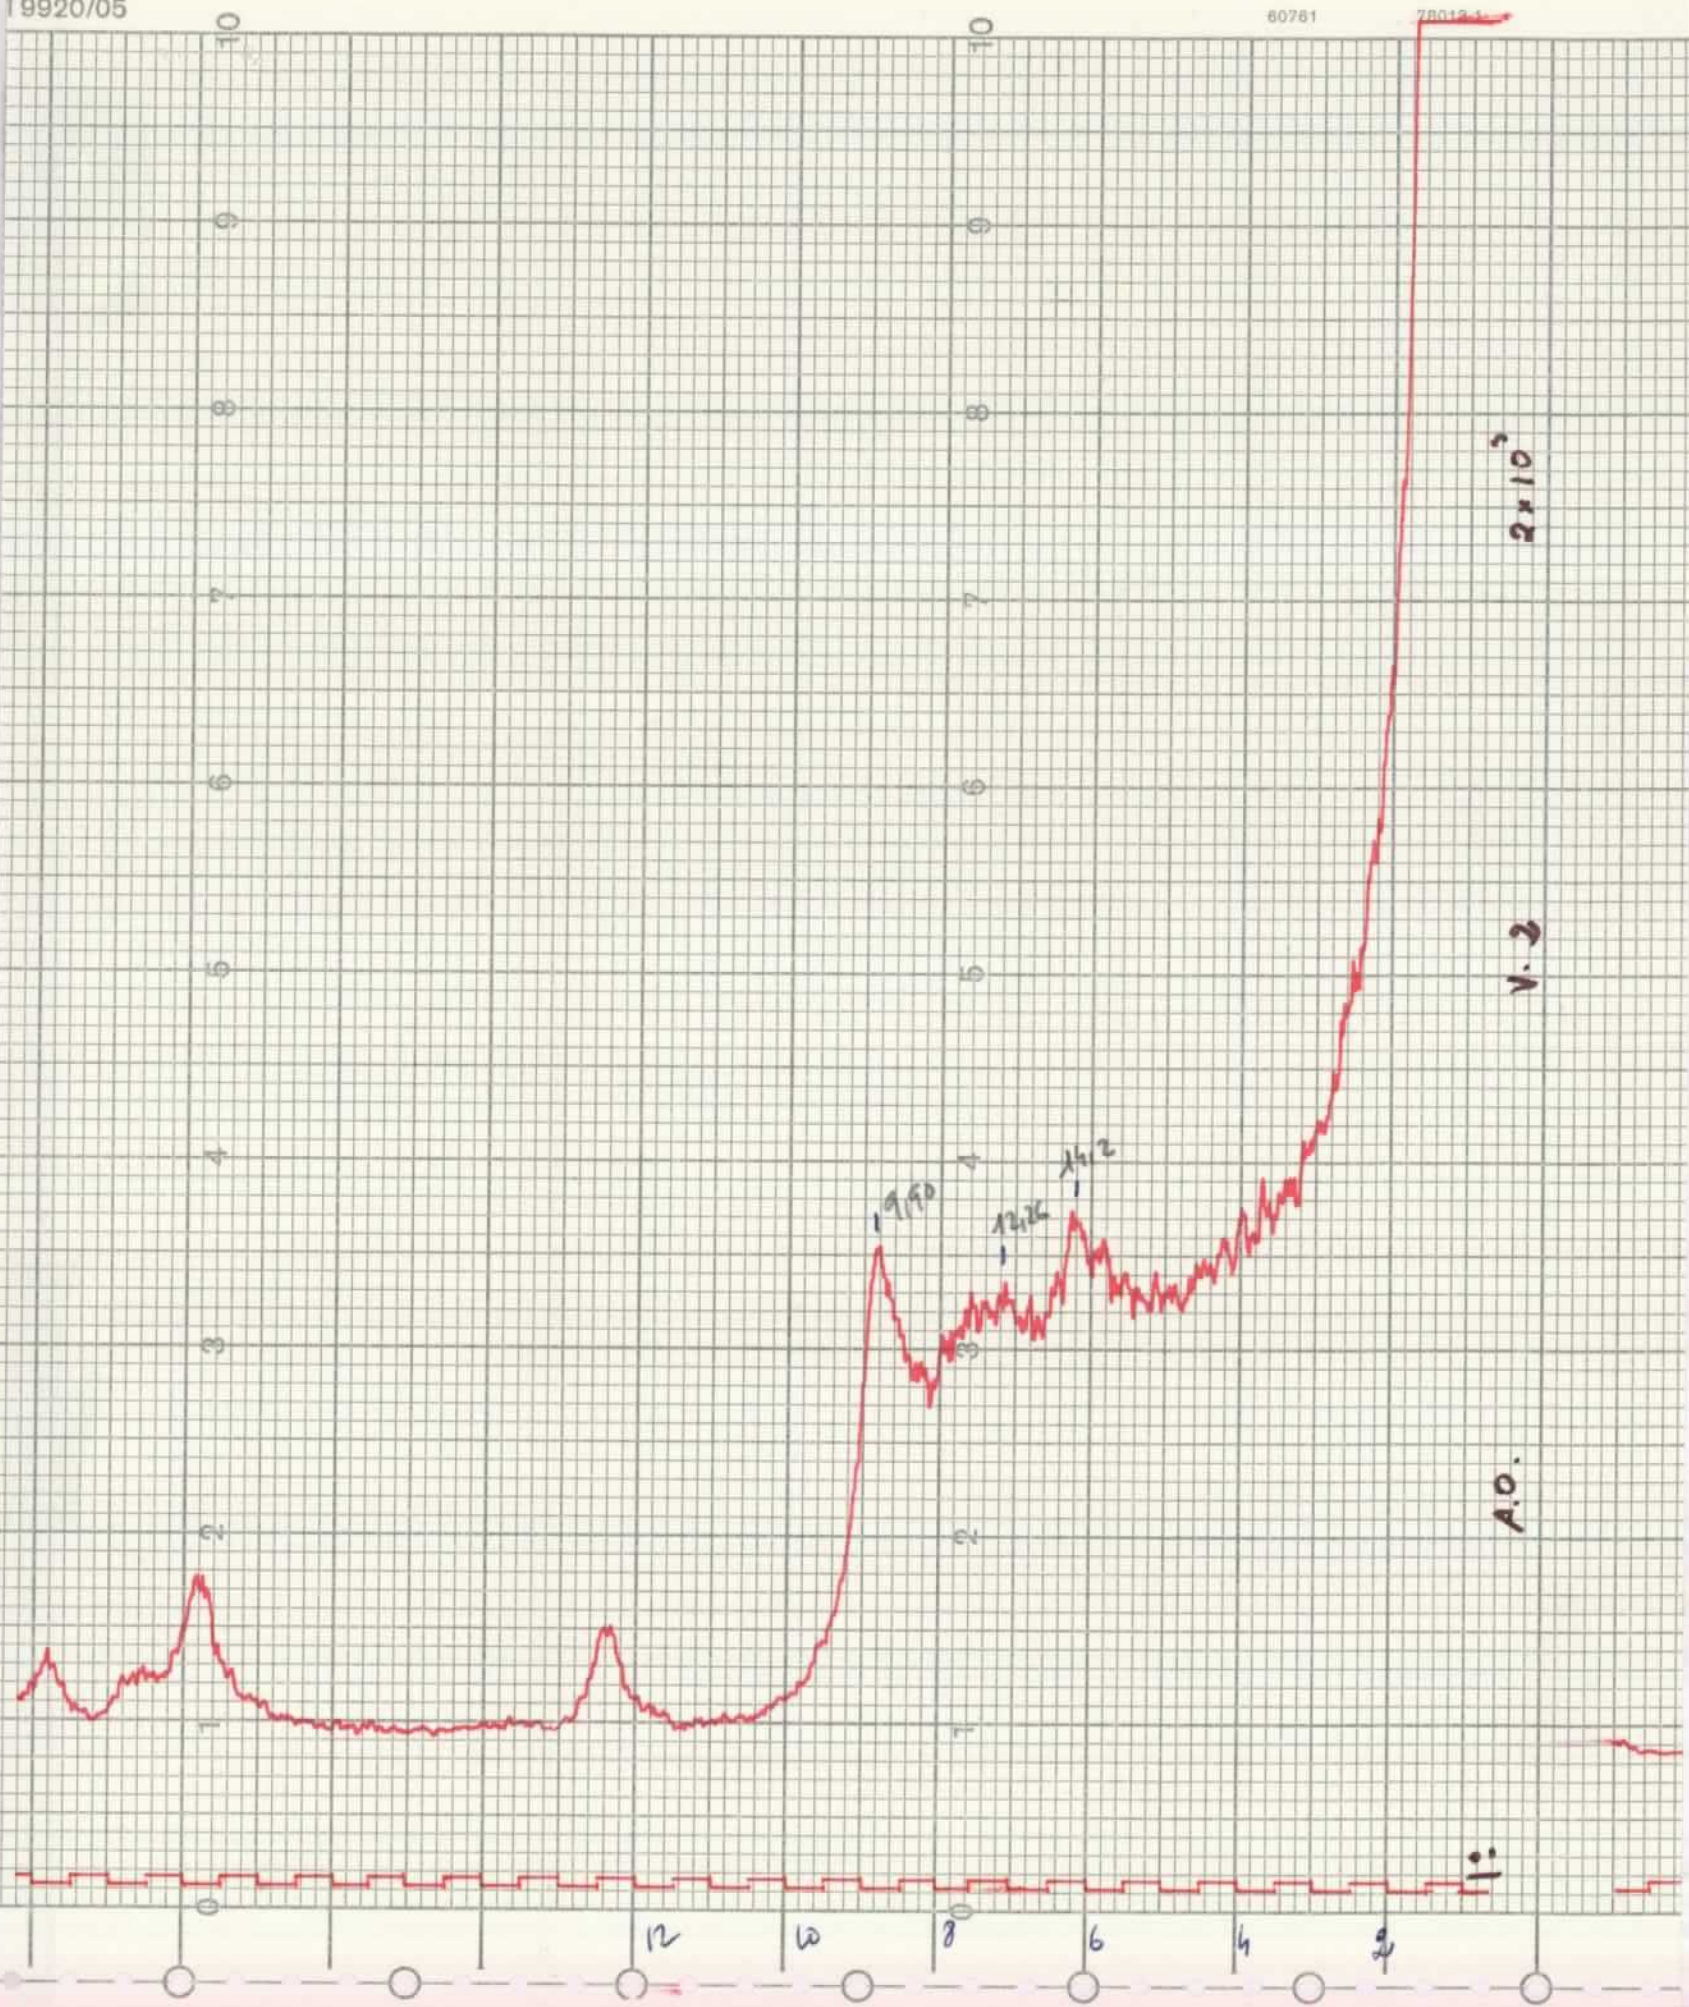

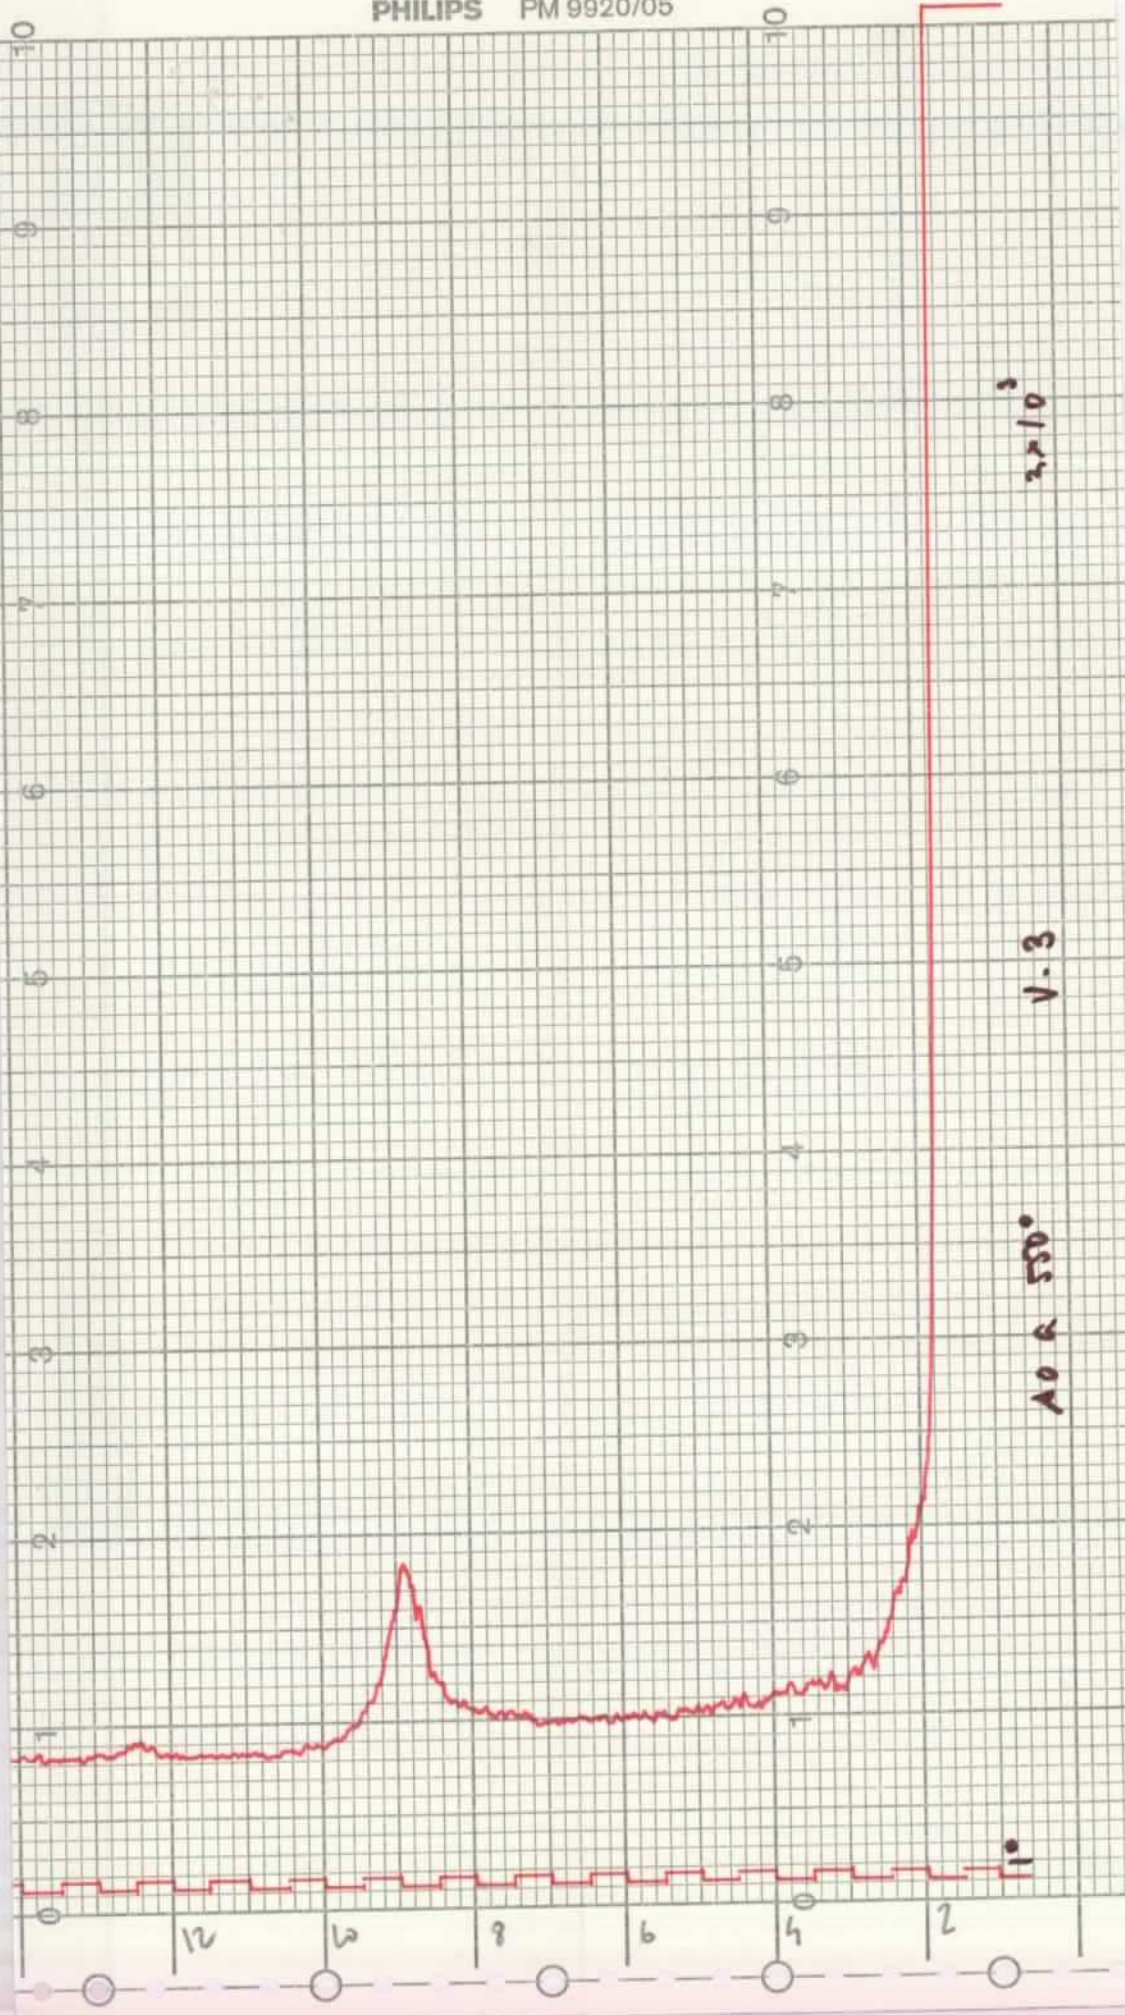





A.D.

V-3

2x10³

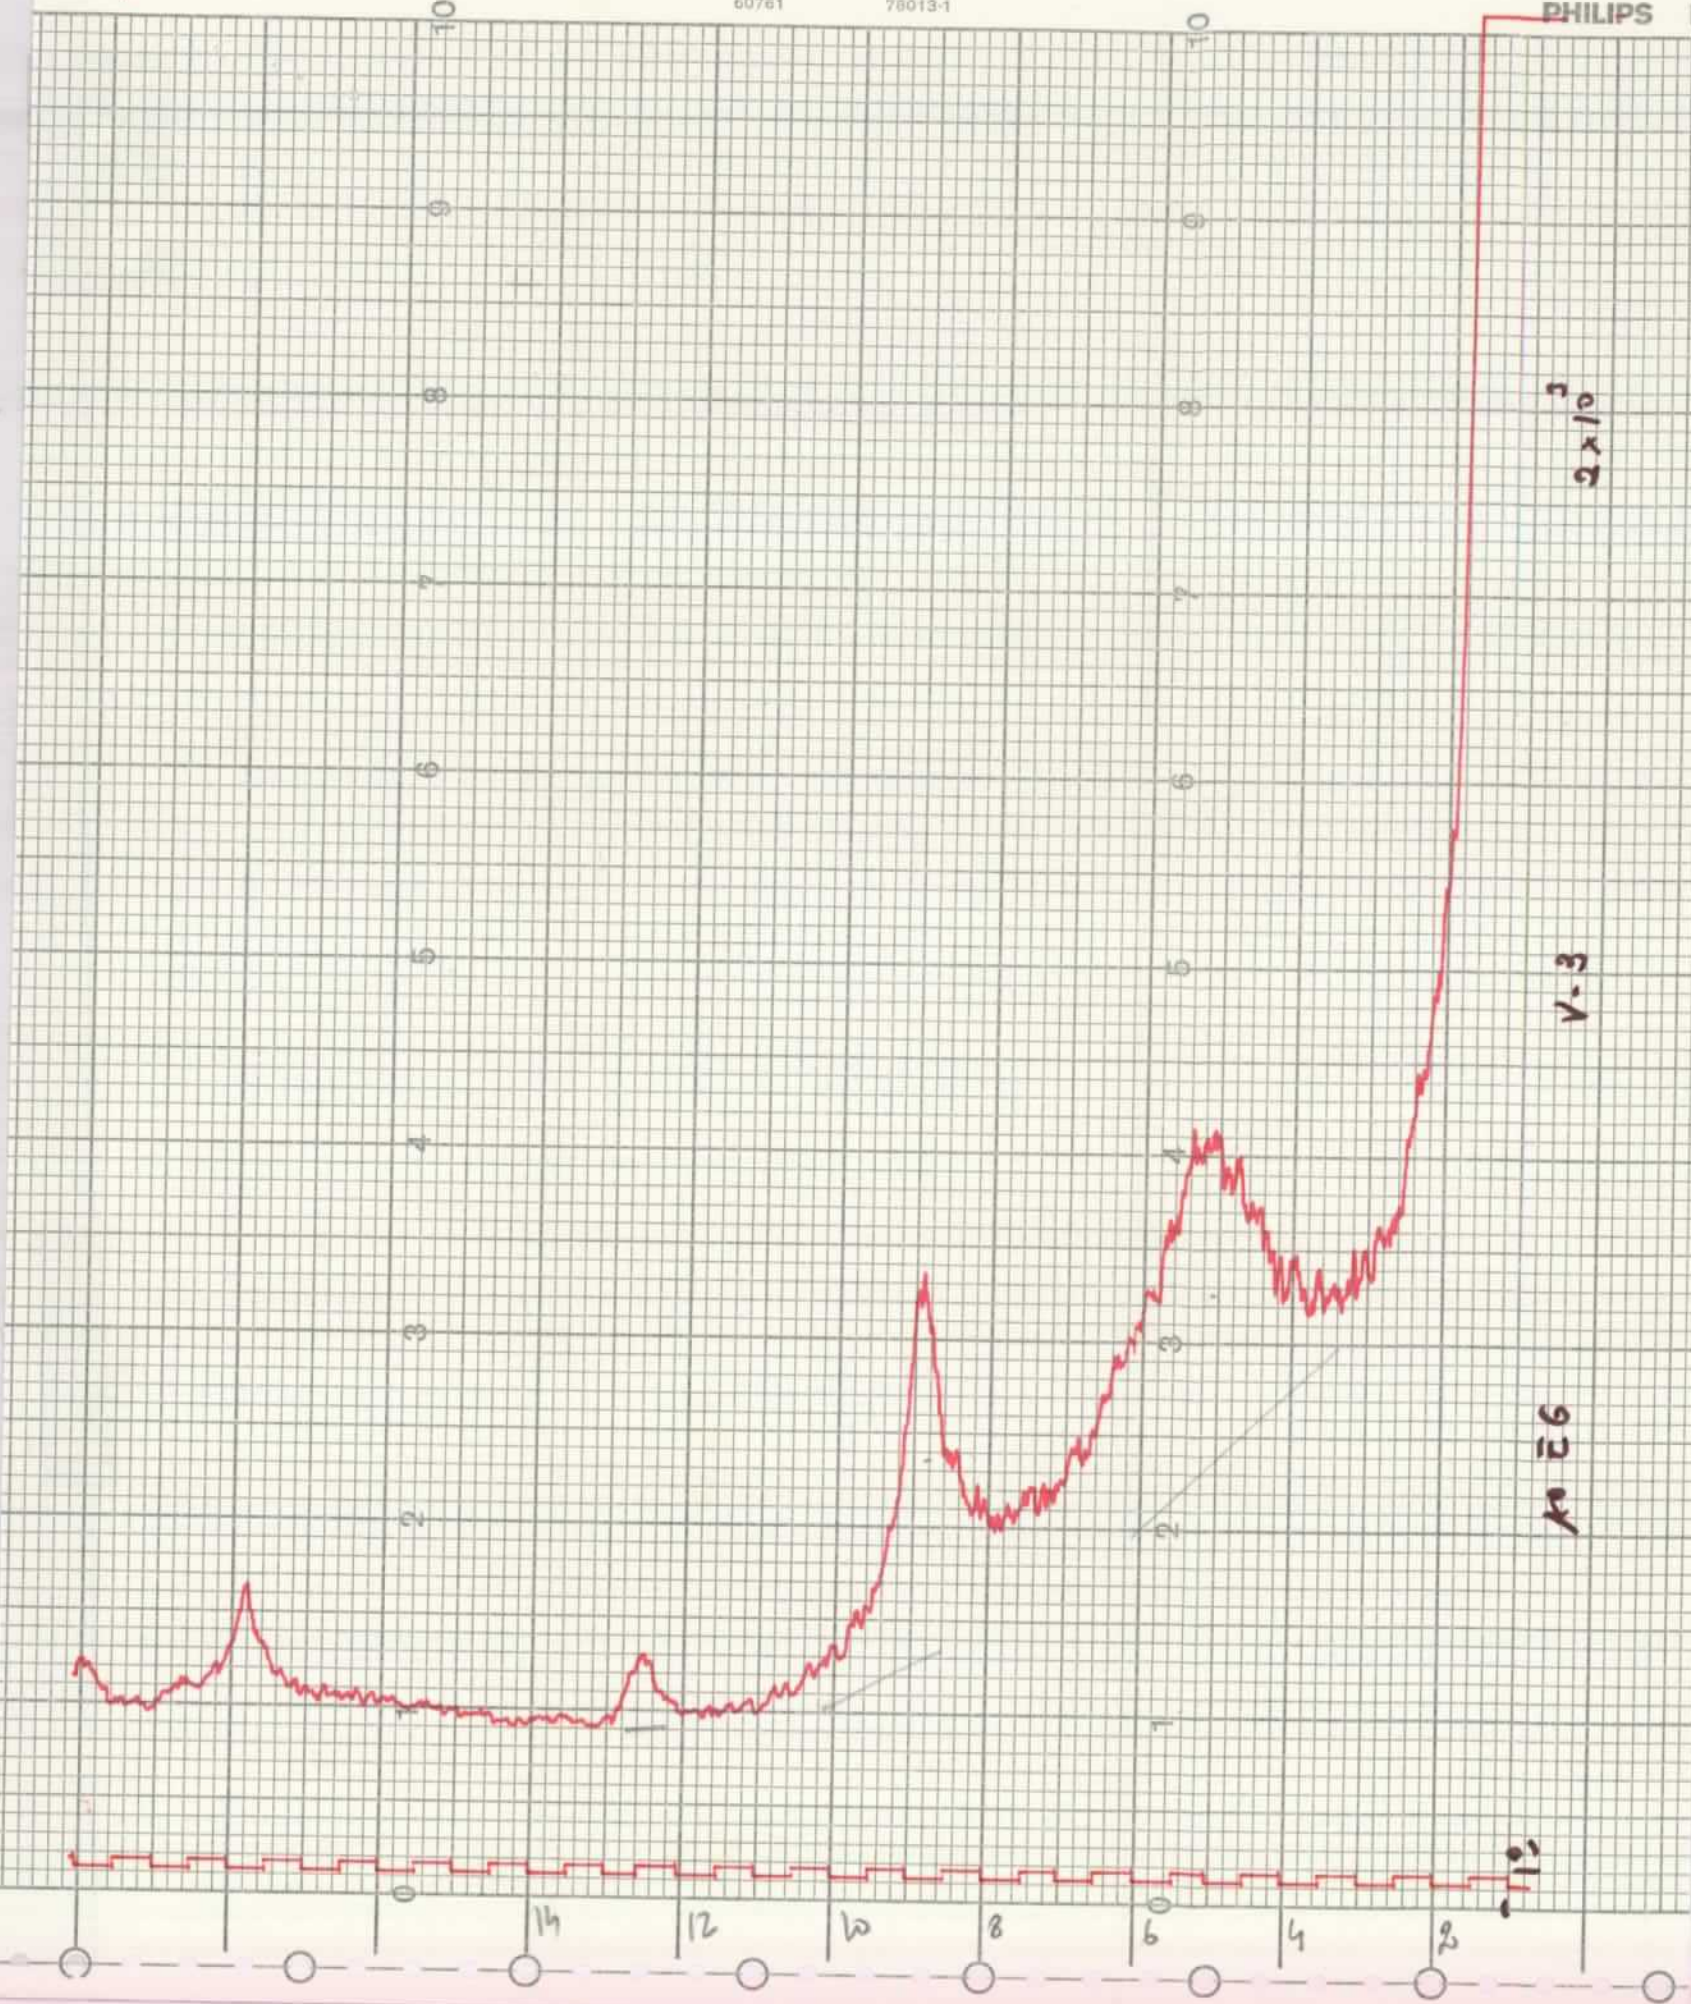



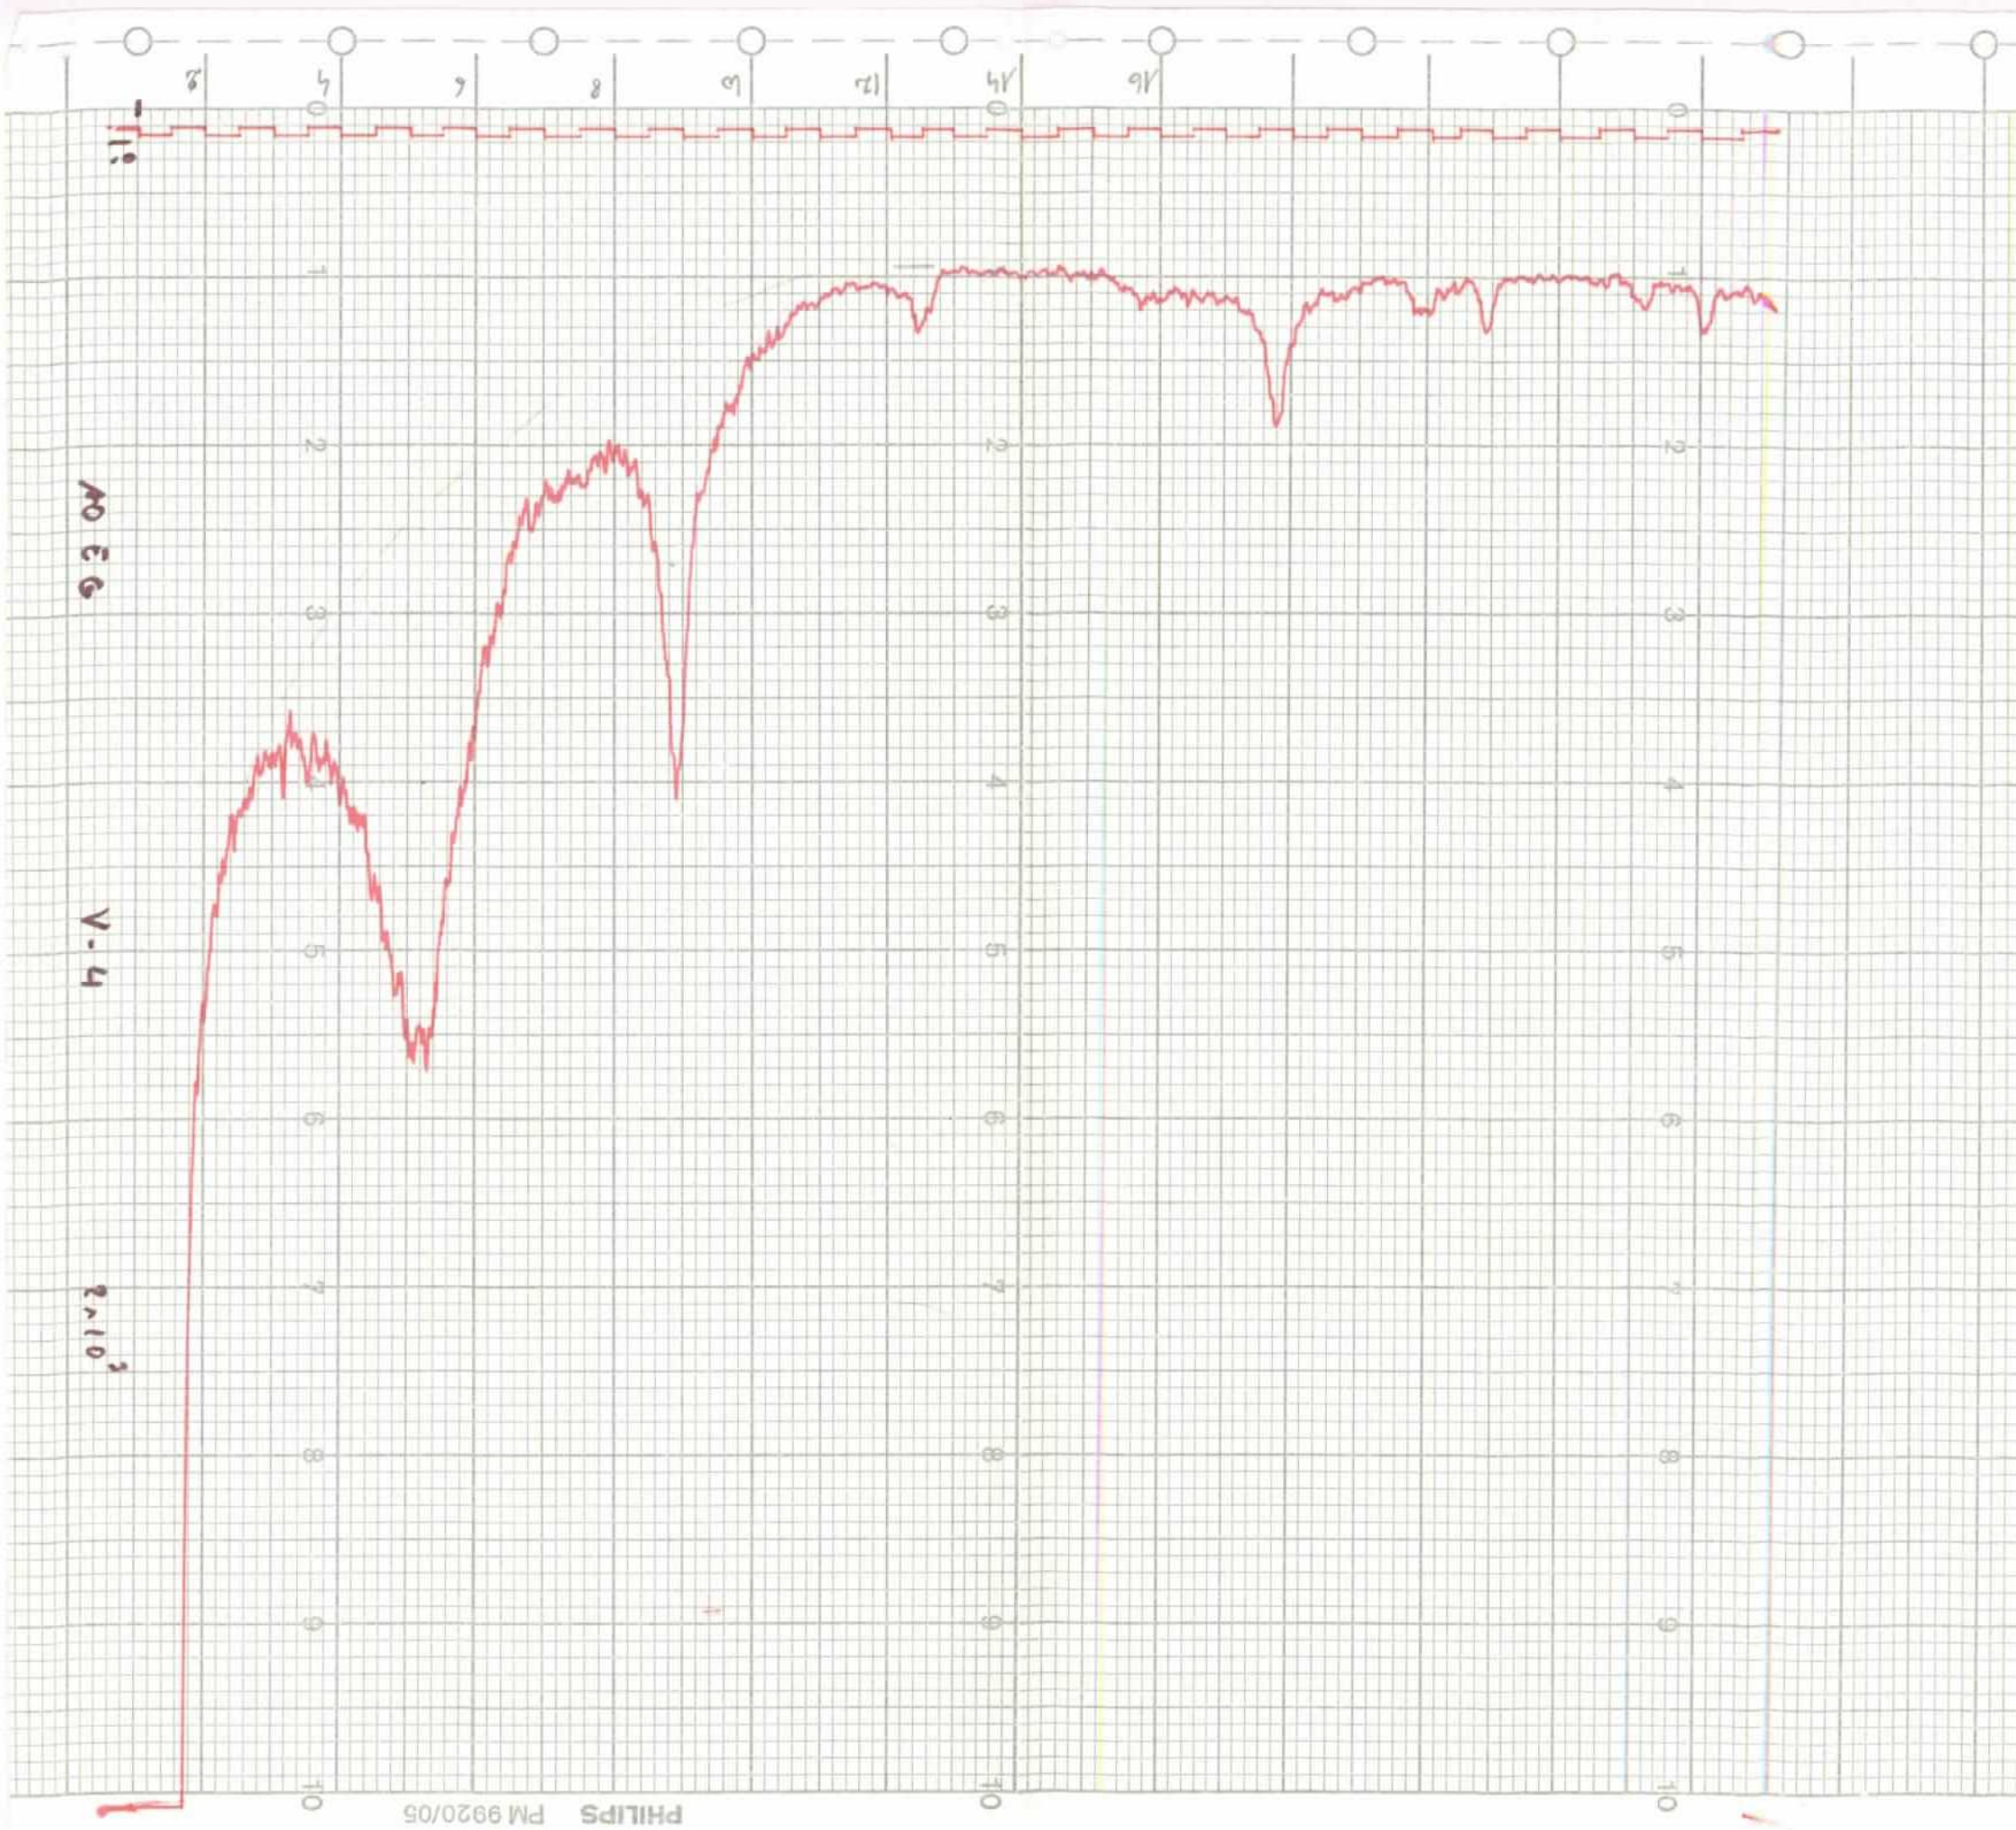

PHILIPS

PM 9920/05

V-4

110

1

2

3

4

5

6

7

8

9

10

1

2

3

4

5

6

7

8

9

10

1

2

3

4

5

6

7

8

9

10

1

2

3

4

5

6


7


8


9

10

19920/05

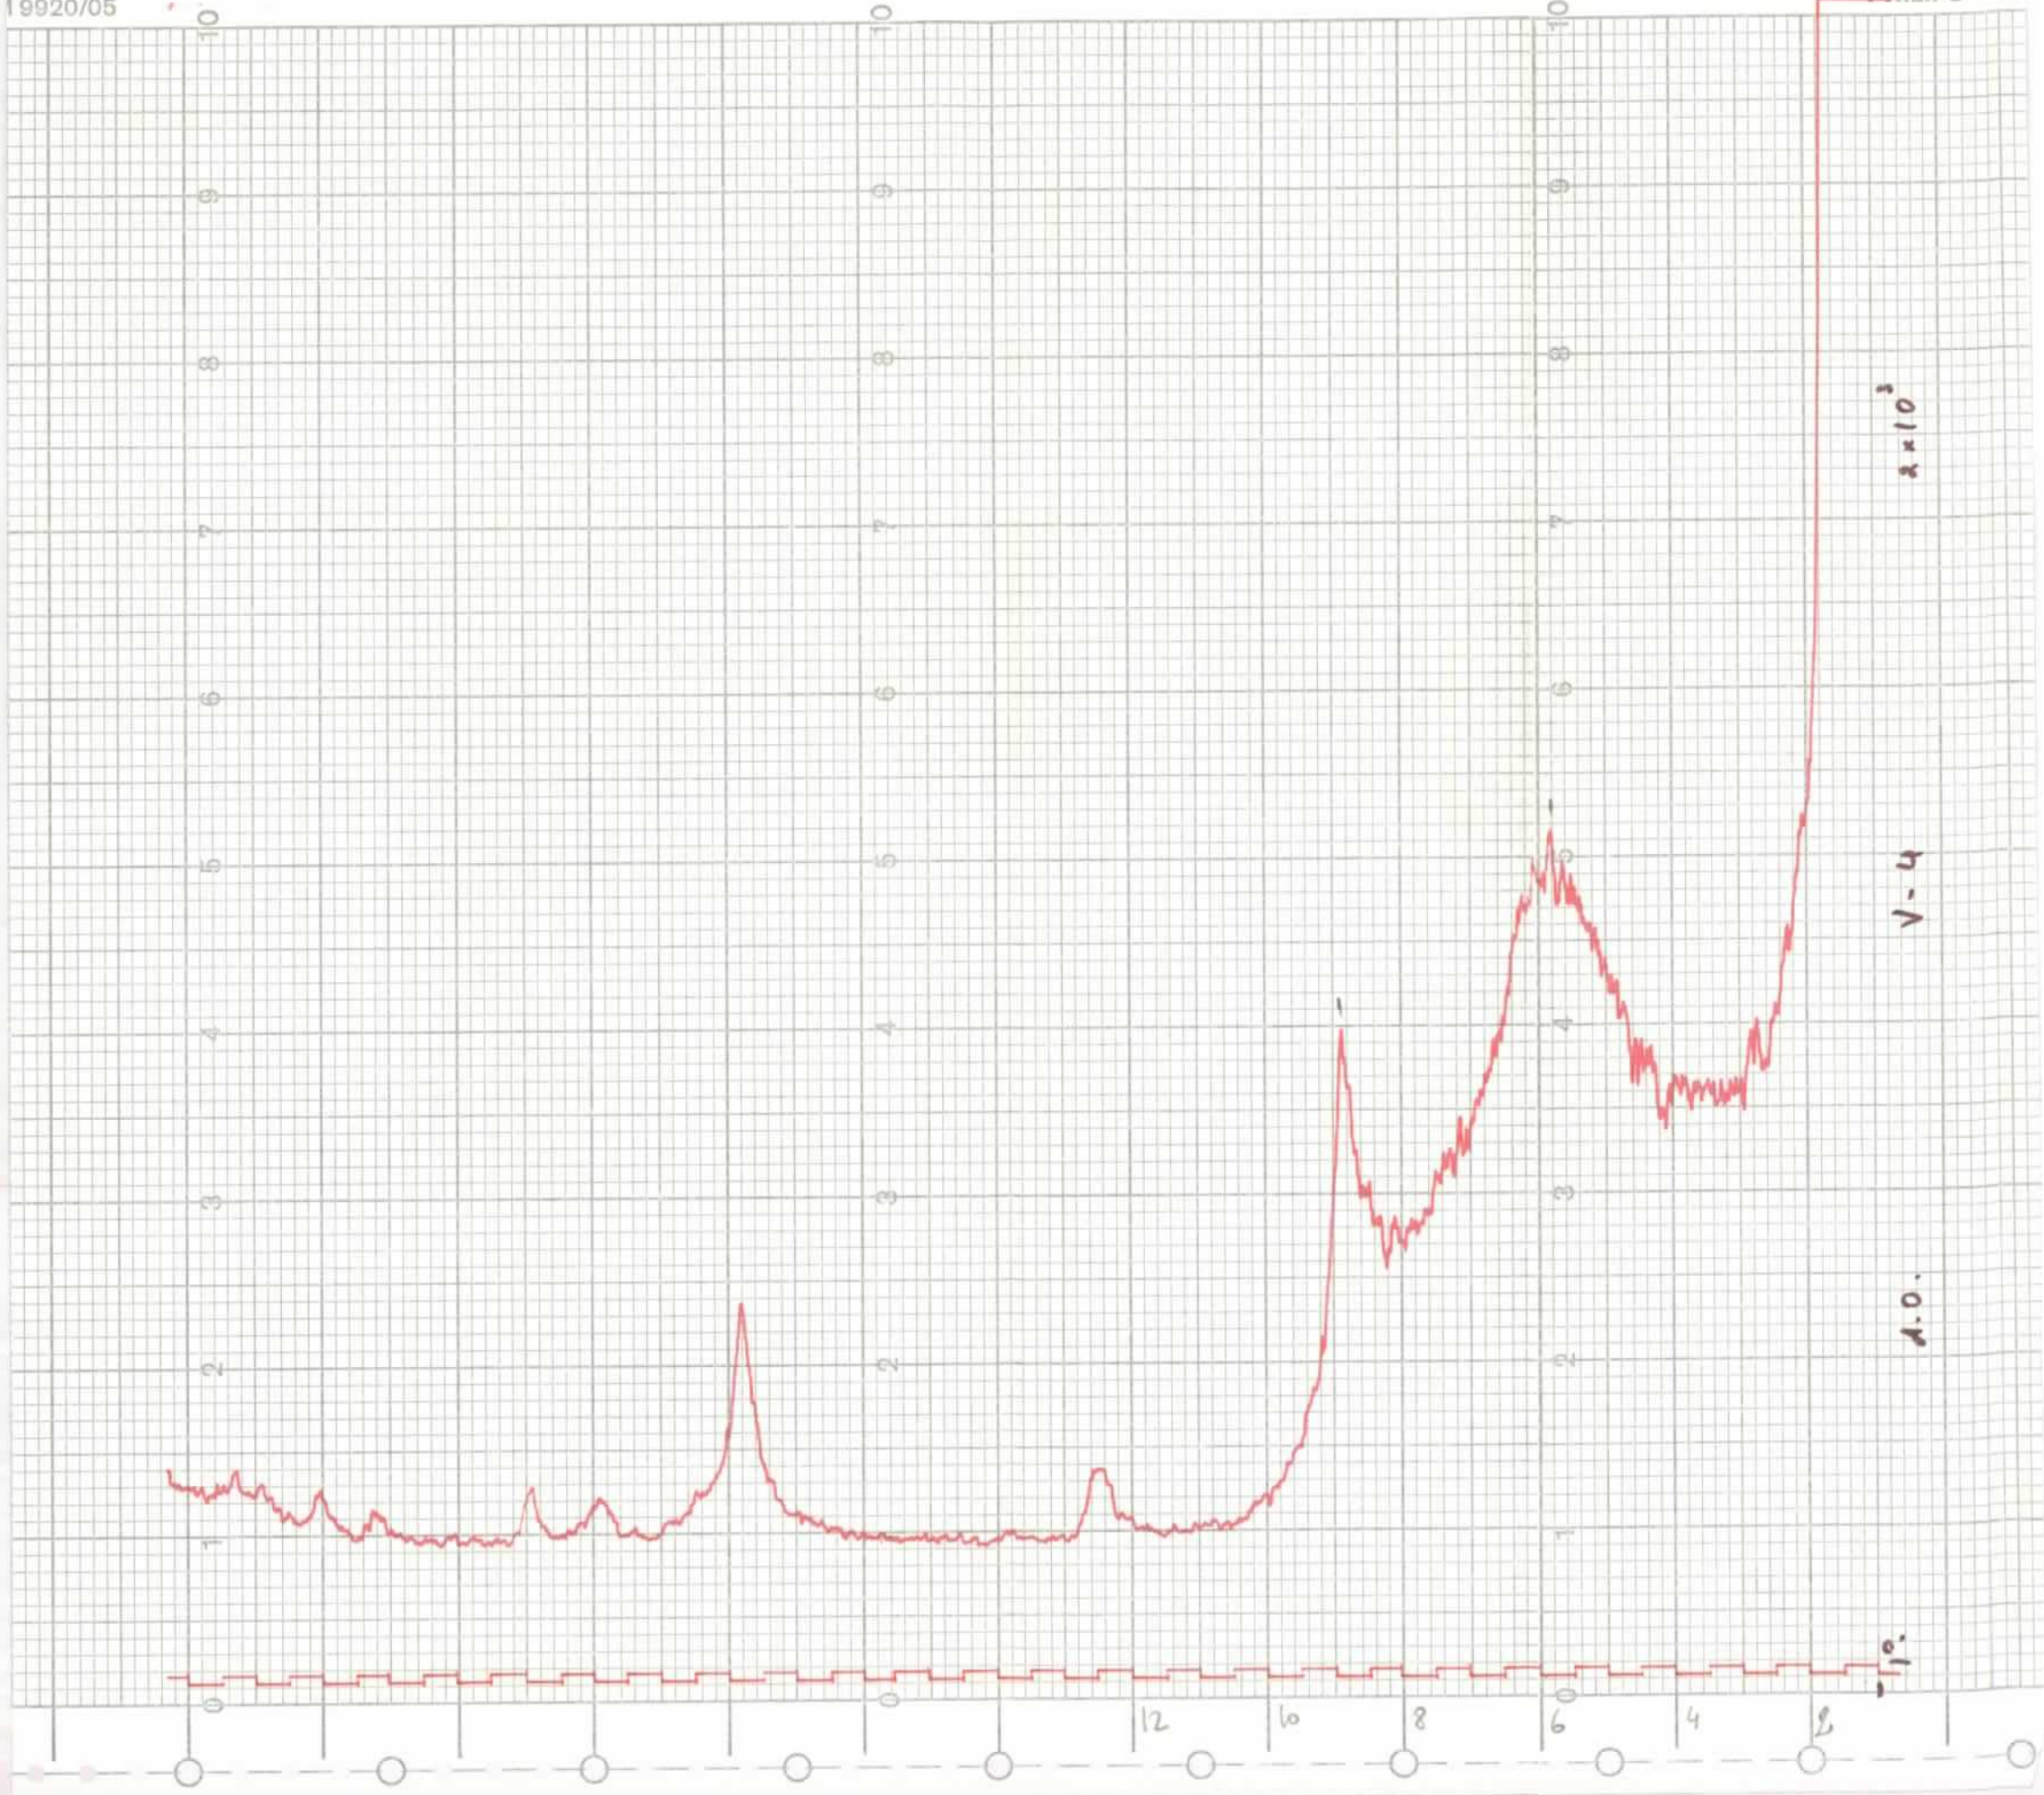

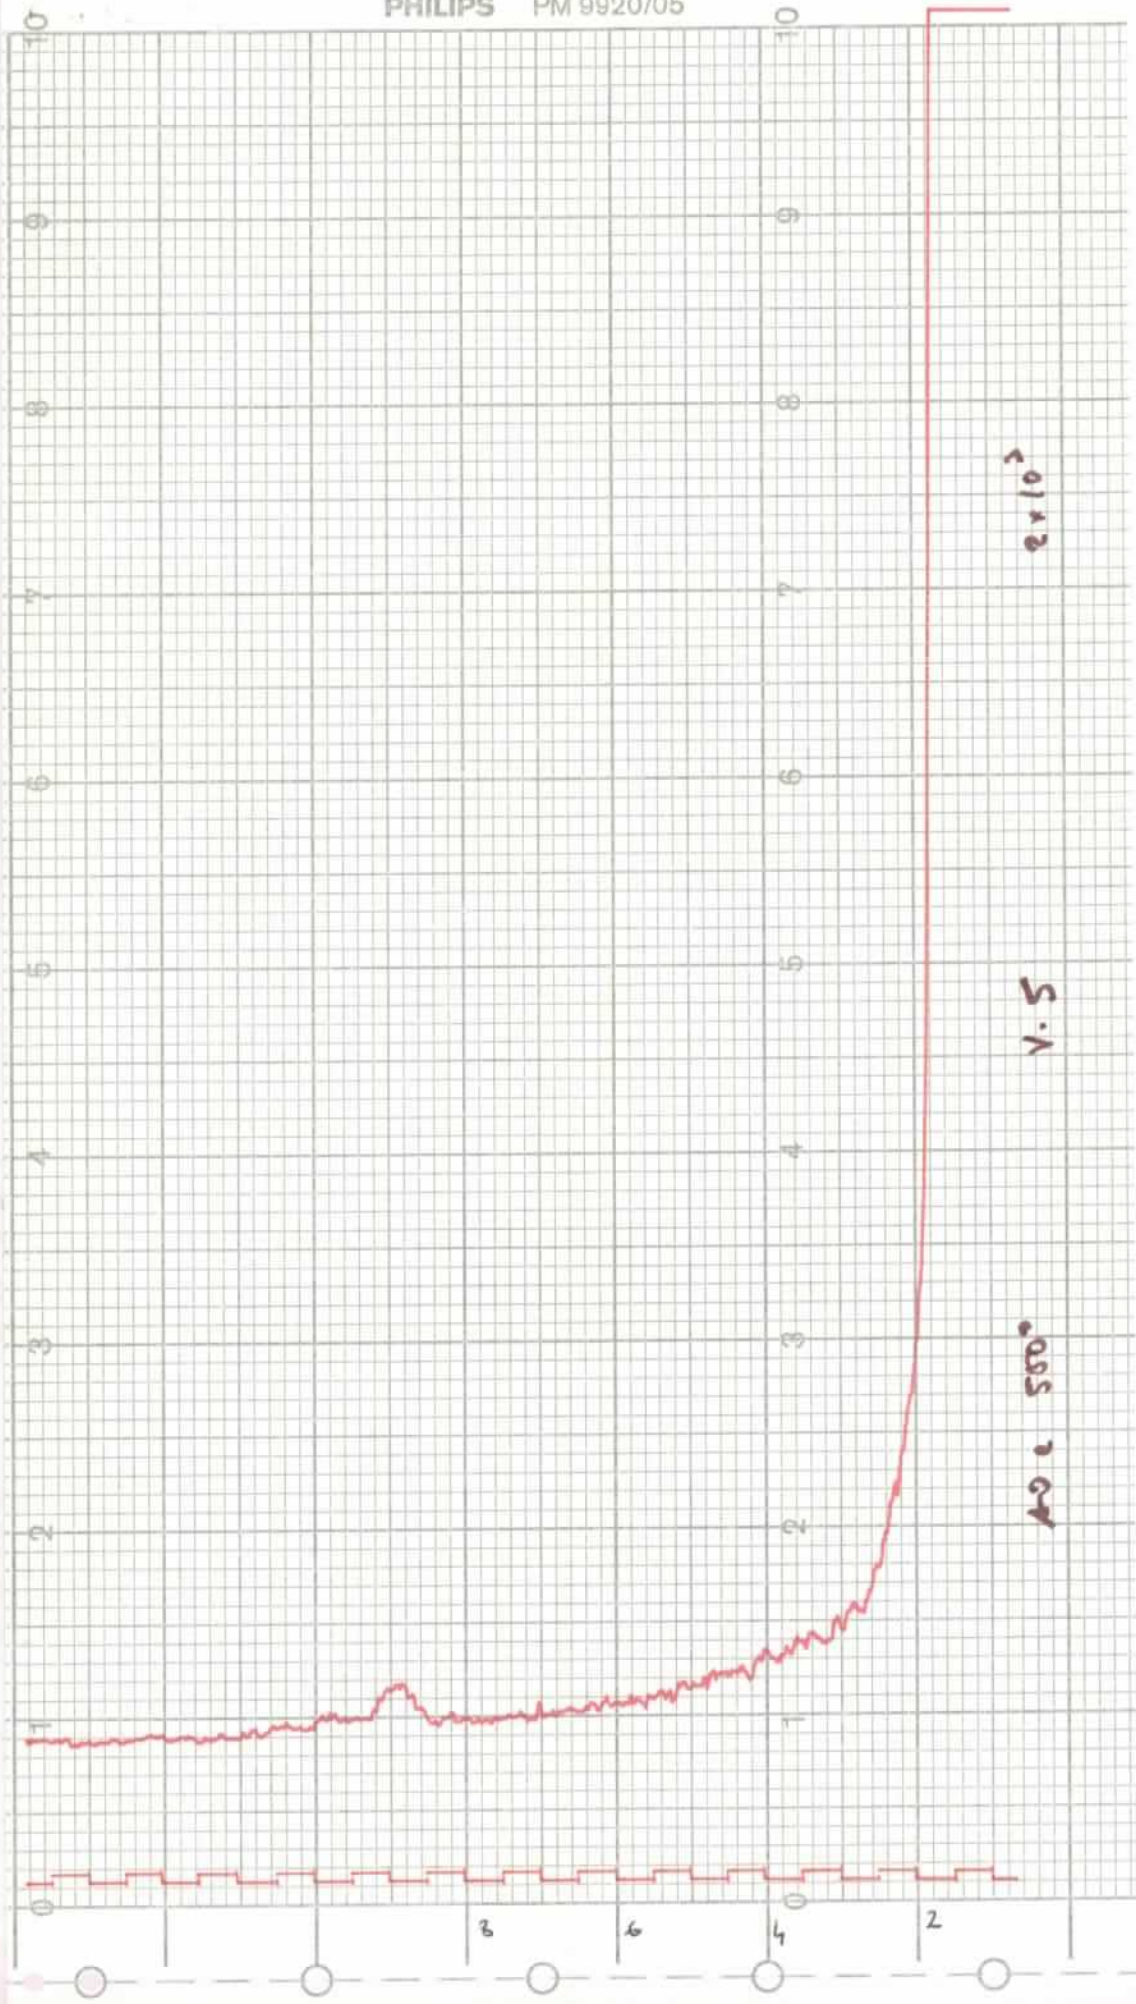

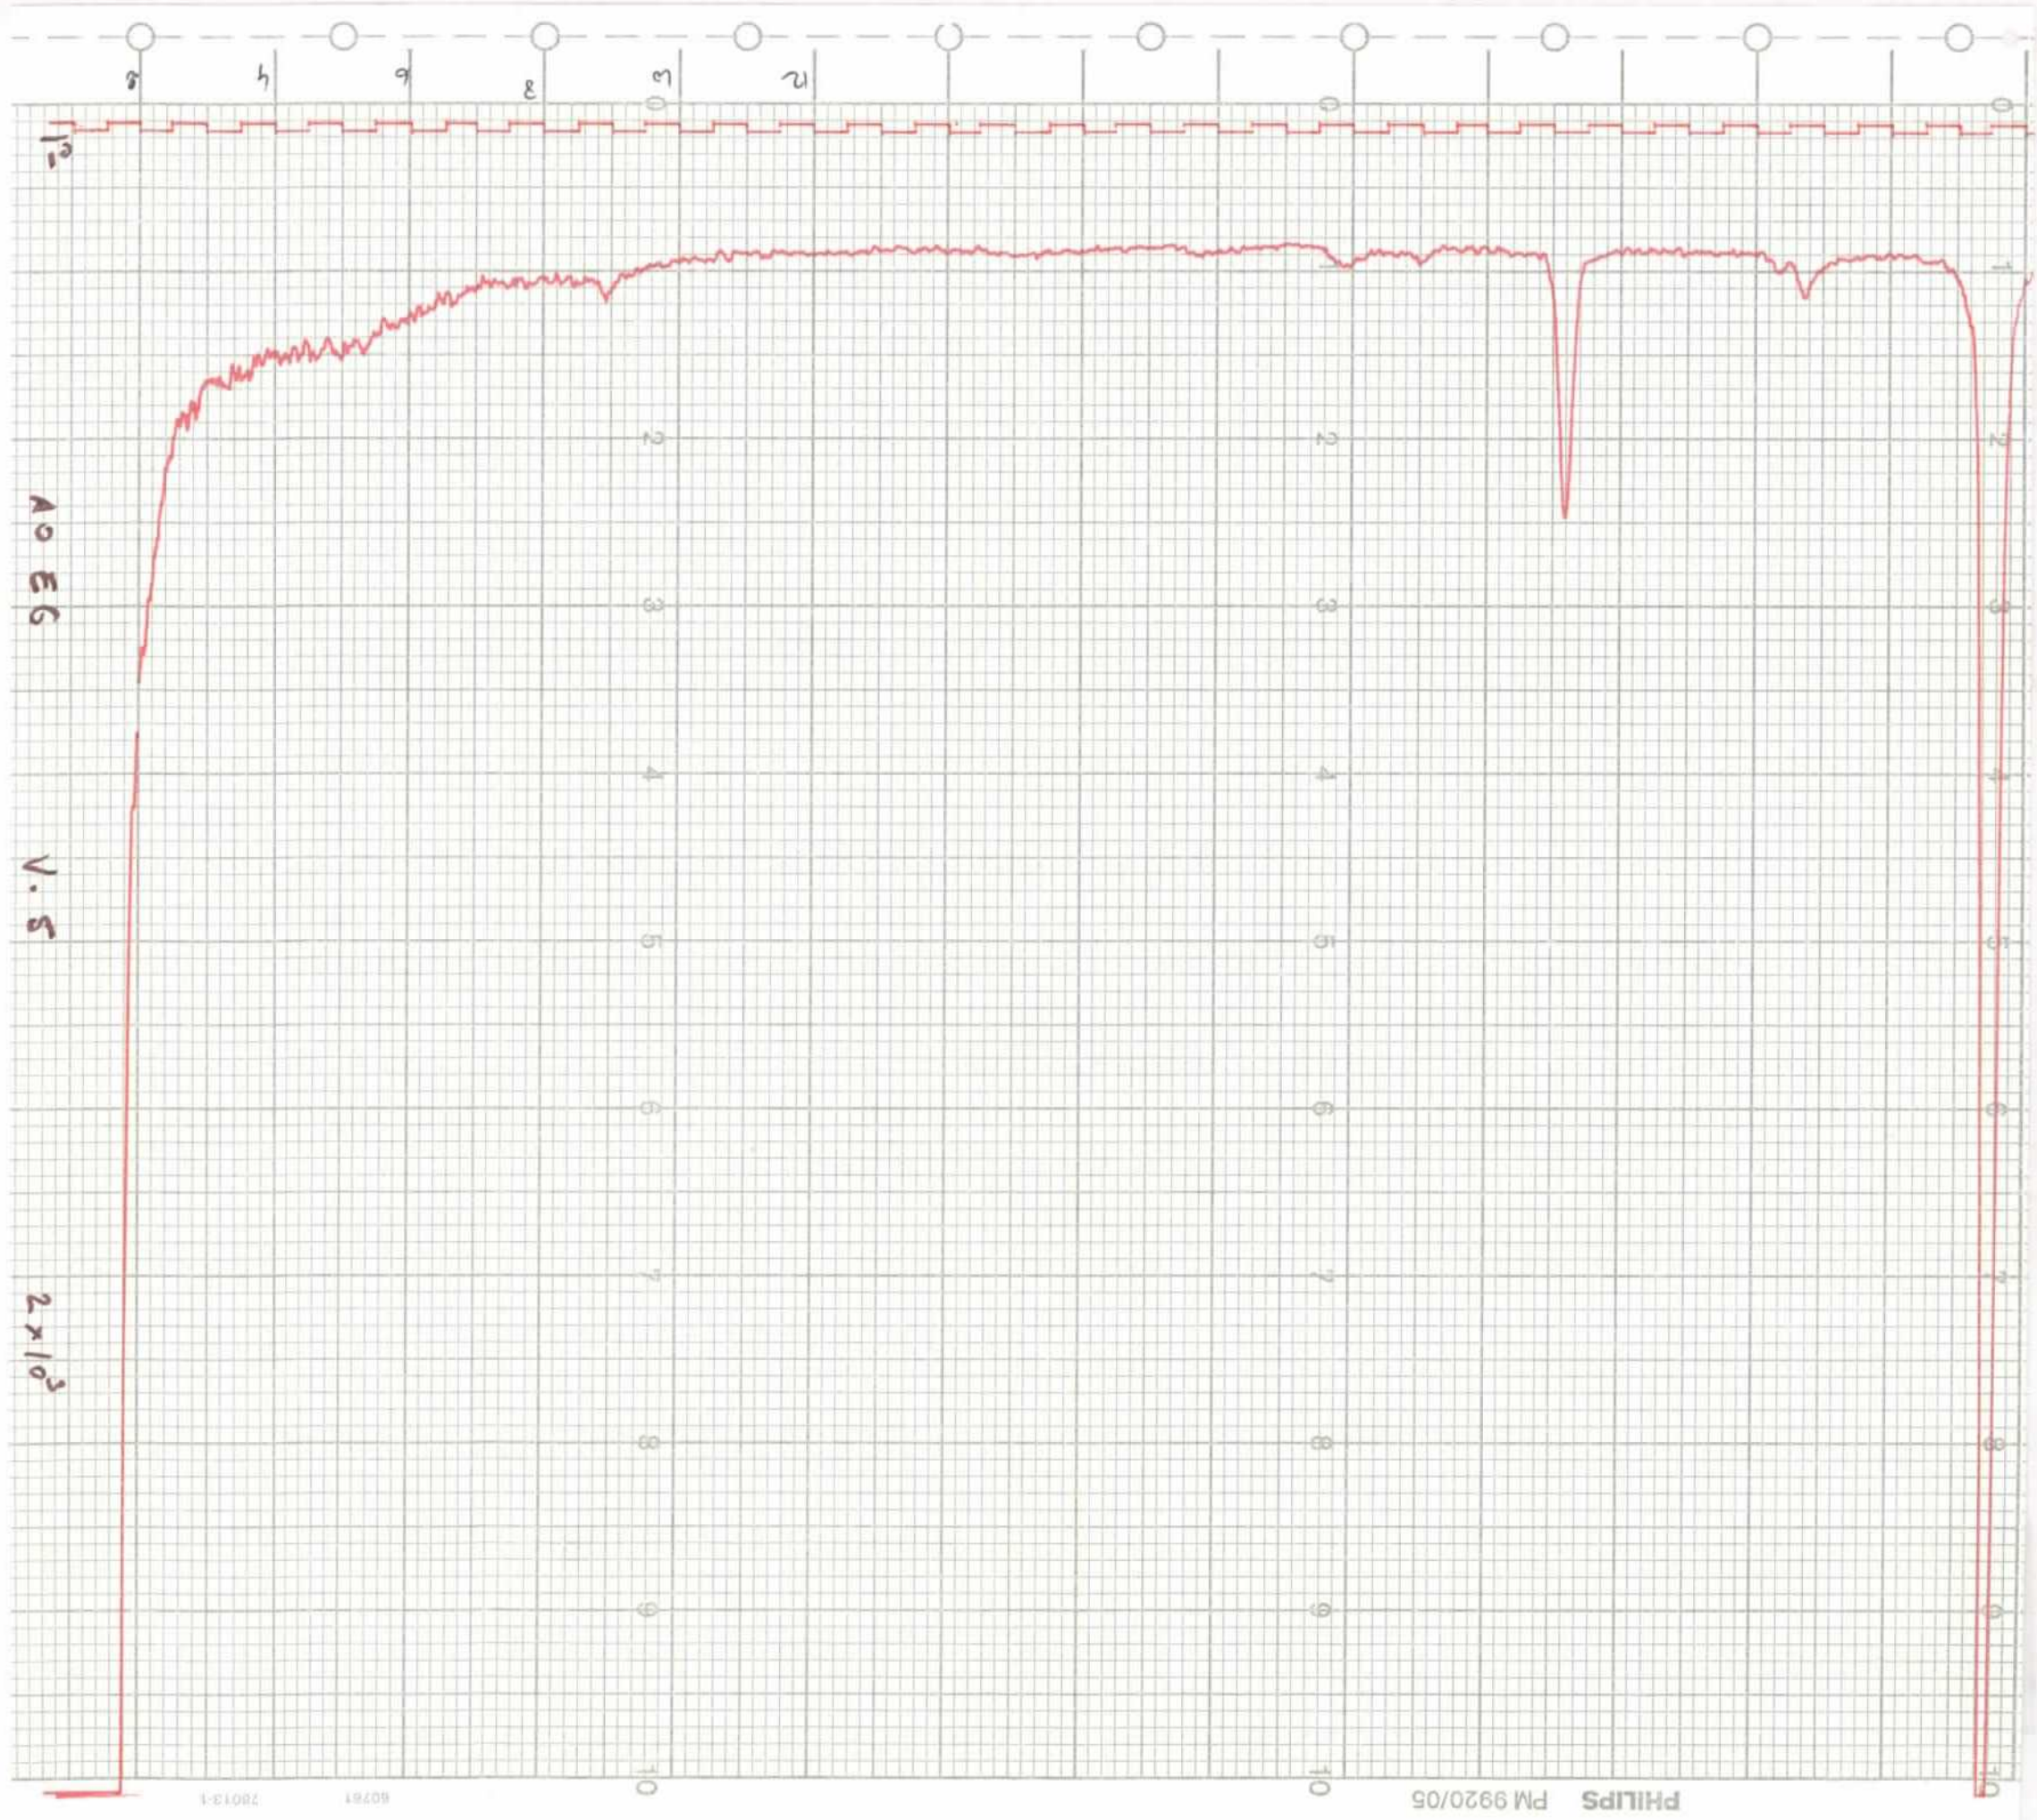

A0 EG


V.S

2×10^3

28013-1

50751

PHILIPS PM 9920/05

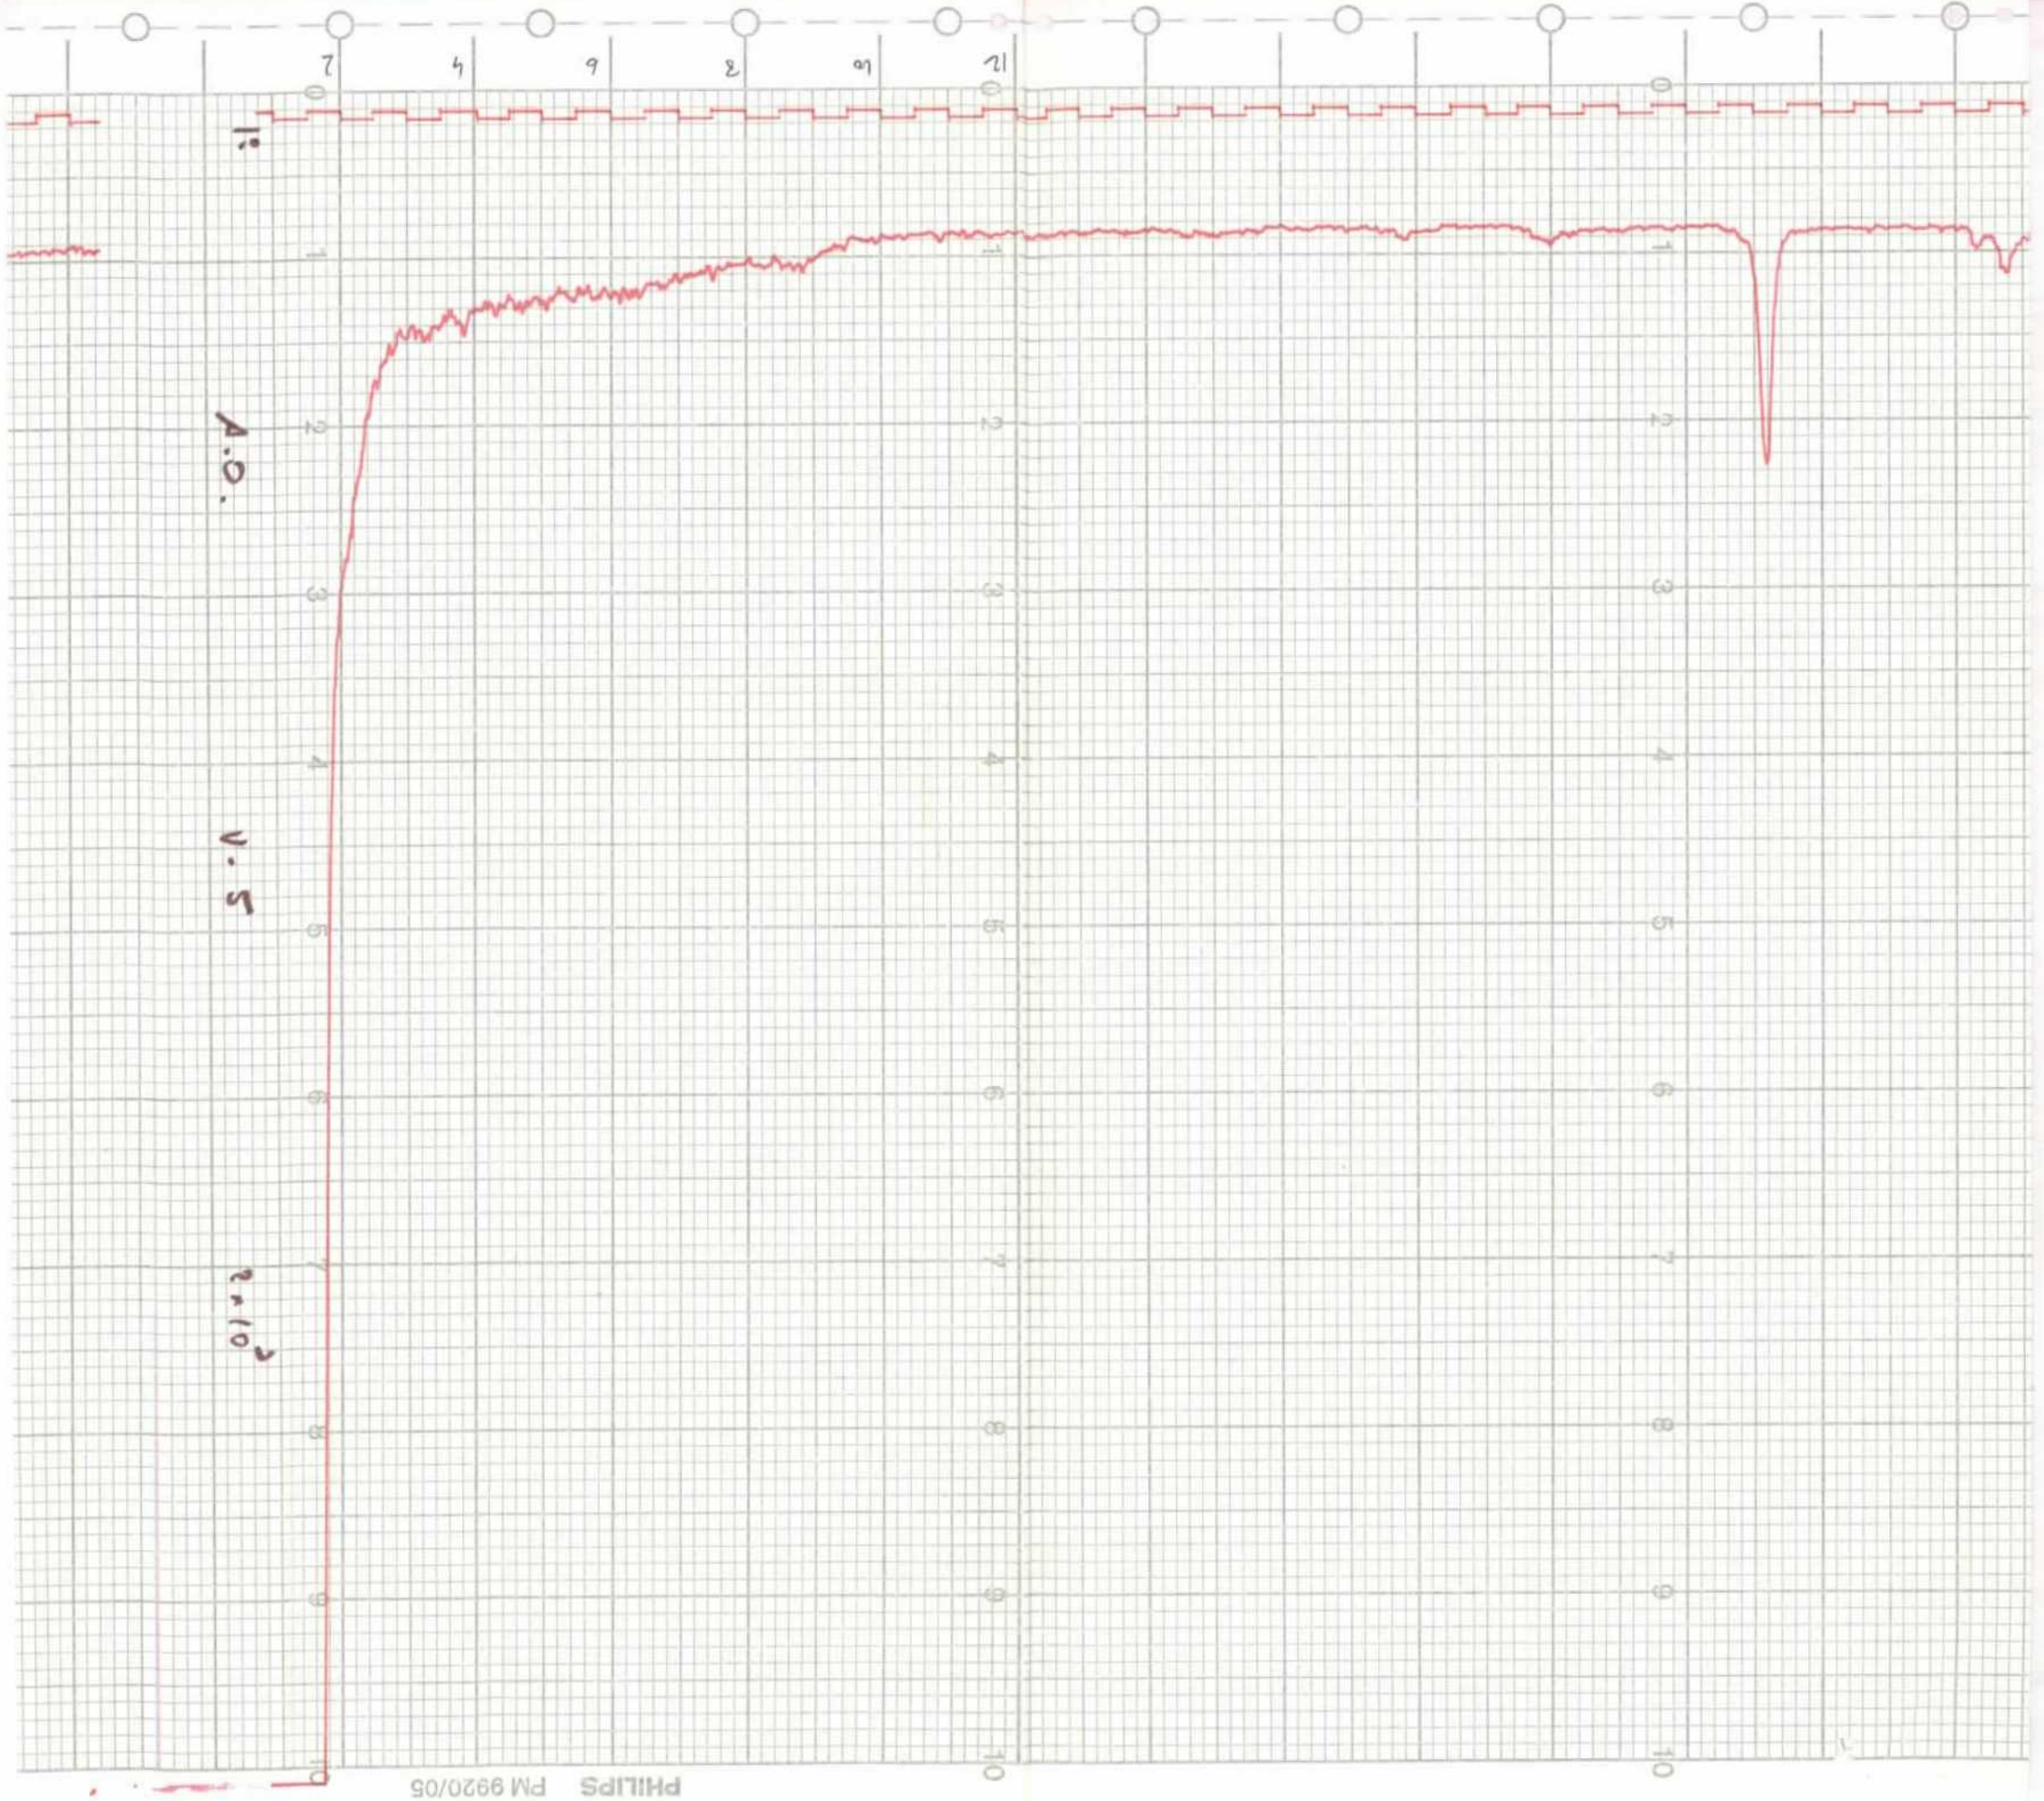



A.O.

V.5

2x10³

19920/05

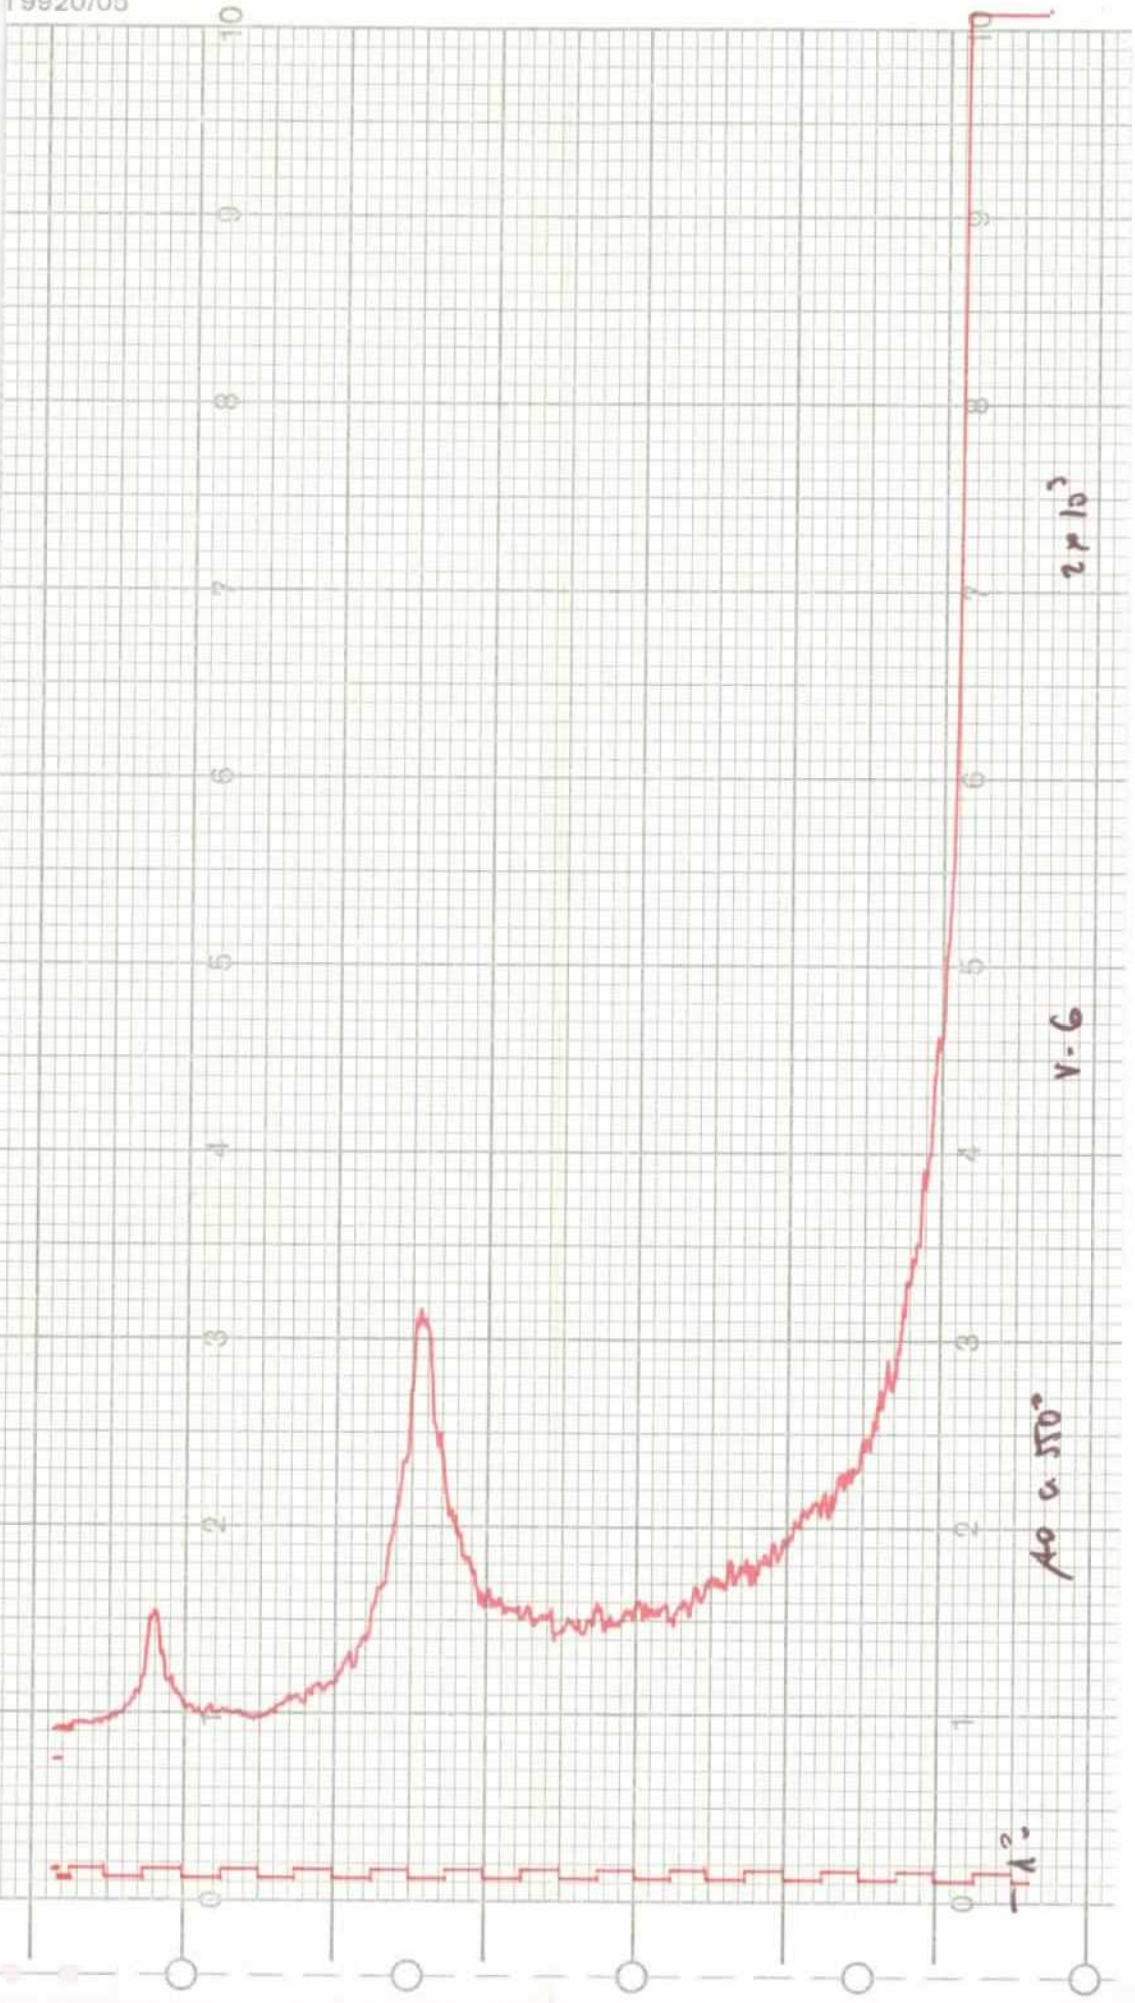

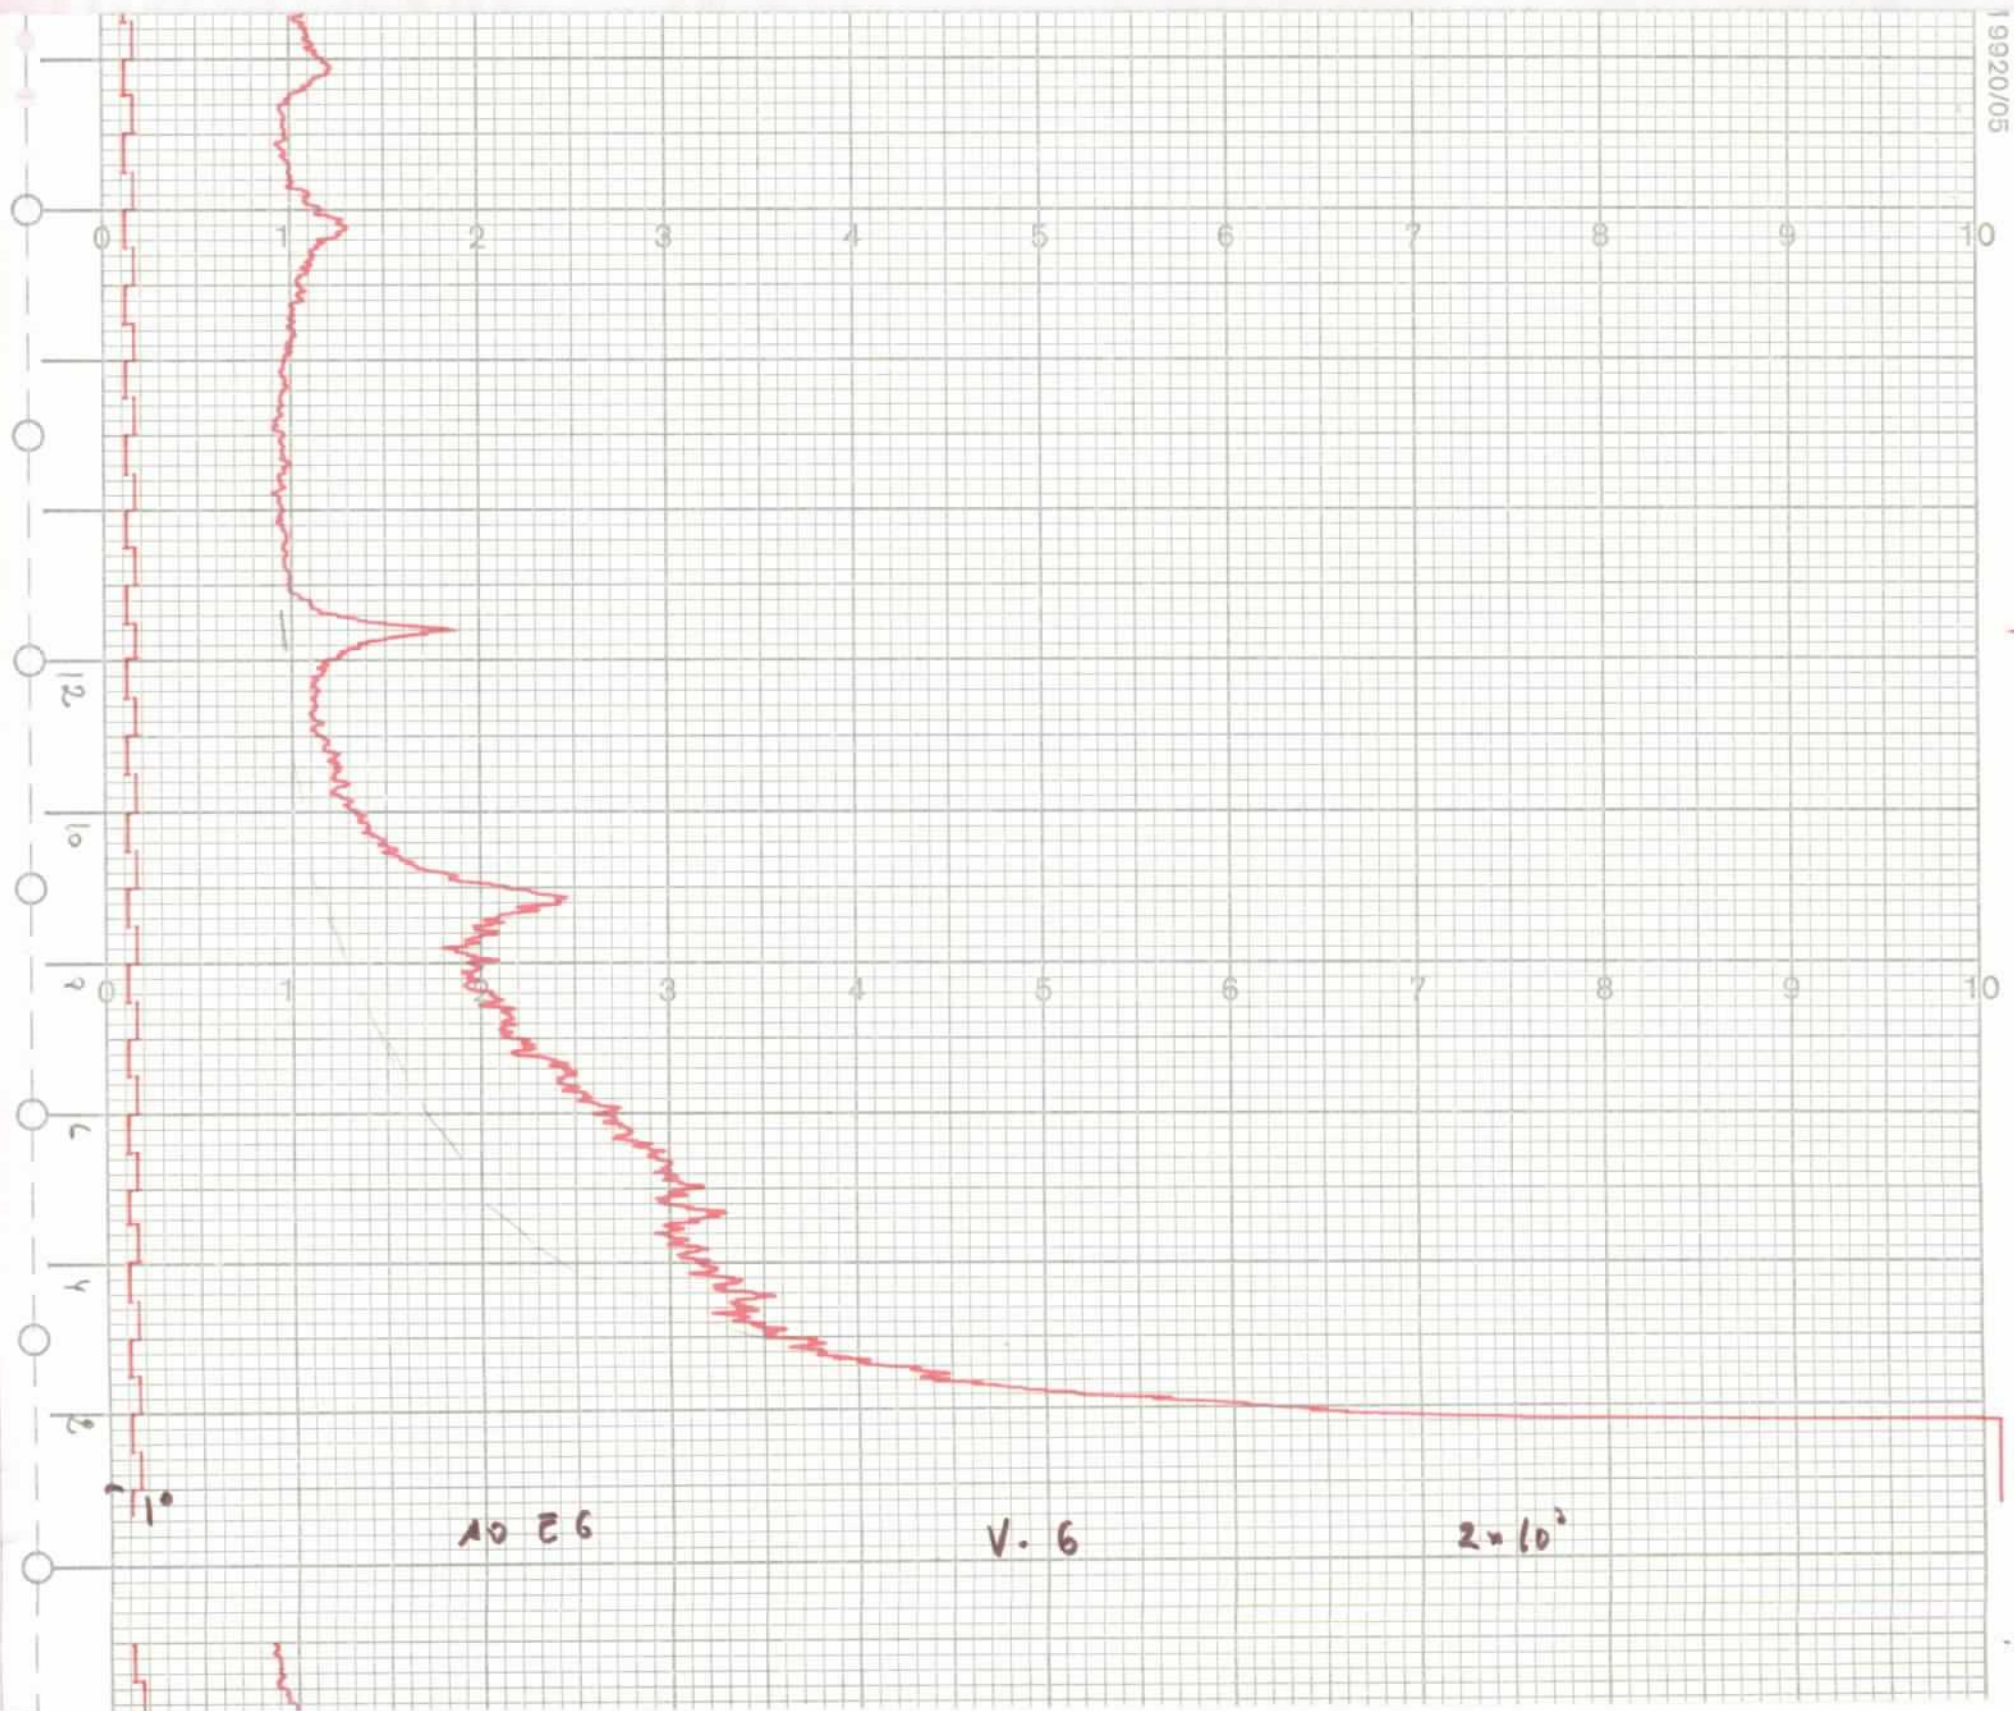

10 E 6

V. 6

2 x 10²

